

## I. SUMMARY

The primary frequency standard NIM5 was used to measure the average fractional frequency difference of the H-maser 57, identified by the clock code 1404857, during an evaluation campaign over 25 days in NOV. 2022. The results are given in table 1, together with the total uncertainties in relating NIM5 to maser 57.

Table 1 Summary of the frequency measurements of H-maser 57 (1404857)

| Period                             | MJD 59884.0 to 59909.0 |
|------------------------------------|------------------------|
| $y_{(H57-NIM5)} [\times 10^{-15}]$ | 66.07                  |
| Duty cycle [%]                     | 99.6%                  |
| $u_A [\times 10^{-15}]$            | 0.38                   |
| $u_B [\times 10^{-15}]$            | 0.90                   |
| $u_{link/lab} [\times 10^{-15}]$   | 0.10                   |
| $u_{total} [\times 10^{-15}]$      | 0.98                   |

The combined total uncertainty  $u_{total}$  is the square sum of the three uncertainties as following:

$$u_{total} = \sqrt{(u_A)^2 + (u_B)^2 + (u_{link/lab})^2} \quad (1)$$

Type A uncertainty  $u_A$  is the statistical uncertainty on the frequency measurement,  $u_B$  is the Type B uncertainty from bias evaluations, and  $u_{link/lab}$  is the uncertainty induced by the link between NIM5 fountain clock and the H-maser 57, which includes the dead time and the phase noise of the link between NIM5 and H-57. All the above uncertainties are calculated at  $1\sigma$ .

## II. Measurement methods

There is no change has been introduced since the previously reported. A summary of the systematic frequency shift evaluations for NIM5 is listed in Table 2. The combined relative Type B uncertainty is approximately  $0.9 \times 10^{-15}$ .

**Table 2** Uncertainty budget of NIM5 in these evaluations.

| Physical Effect | Bias [ $\times 10^{-15}$ ] | Uncertainty [ $\times 10^{-15}$ ] |
|-----------------|----------------------------|-----------------------------------|
|-----------------|----------------------------|-----------------------------------|

|                                  |        |      |
|----------------------------------|--------|------|
| 2nd order Zeeman                 | 73.21  | 0.2  |
| Collisional shift                | -3.03* | 0.1  |
| Microwave interferometric Switch | 0.0    | 0.6  |
| Microwave leakage                | 0      | <0.1 |
| DCP                              | 0.0    | 0.6  |
| Microwave spectral impurities    | 0.0    | 0.1  |
| Blackbody radiation              | -16.22 | 0.1  |
| Gravitational red shift          | 11.77  | 0.1  |
| Majorana transition              | 0.0    | 0.1  |
| Light shift                      | 0.0    | <0.1 |
| Rabi and Ramsey pulling          | 0.0    | <0.1 |
| Cavity pulling                   | 0.0    | <0.1 |
| Collision with background gases  | 0.0    | <0.1 |
| Total                            | 65.73* | 0.9* |

\* The collision shift is calculated at low density.

The dead time distribution during the report period is shown in the figure 1:

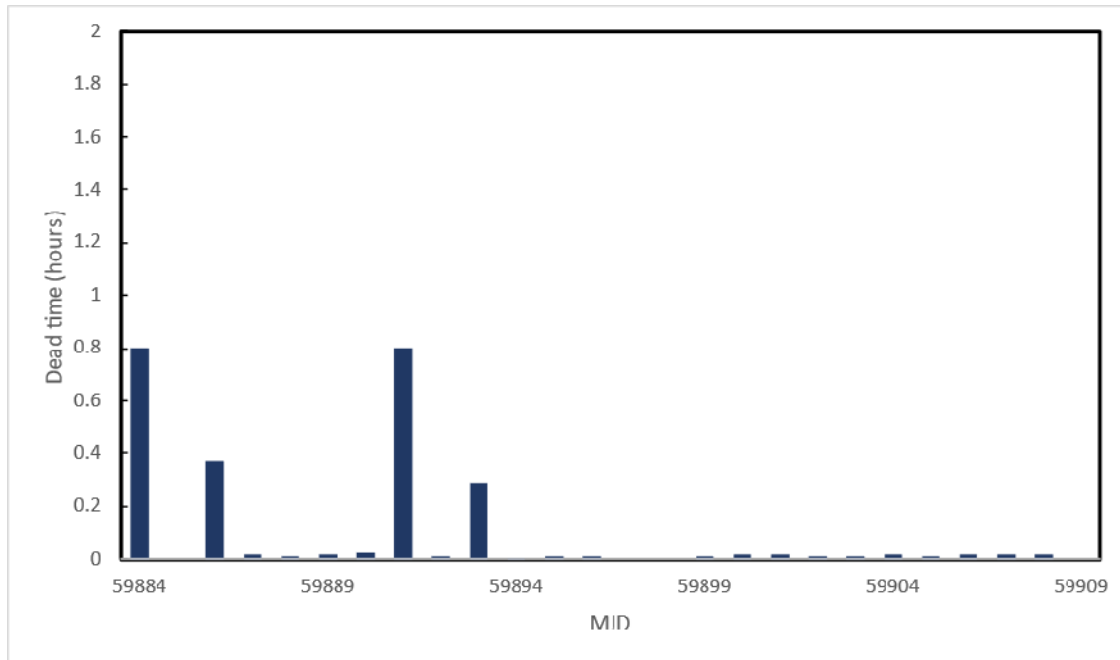


Figure 1 Dead time distributions in NOV., 2022 report period.