

# Frequency evaluation of **HM1405624** by **KRISS-Yb1** for the period **MJD 61219 to MJD 61249**

The frequency of the hydrogen maser HM1405624 was evaluated during the period **MJD 61219 – 61249 (Jun. 28, 2026 – Jul. 28, 2026)** using the Yb optical lattice frequency standard KRISS-Yb1 and an optical frequency comb. The KRISS-Yb1 absolute frequency was assumed to be the most recently recommended BIPM value: 518,295,836,590,863.632 Hz [1]. The results of the evaluation are given in the table below. More details of the KRISS-Yb1 operation and the uncertainty budget can be found in Ref. 2.

## 1. Results

(a) Results of the frequency evaluation in  $1 \times 10^{-16}$

| Period (MJD)  | $\gamma(\text{HM}_{1405624} - \text{KRISS-Yb1})$ | $u_A$ | $u_B$ | $u_{A/\text{Lab}}$ | $u_{B/\text{Lab}}$ | $u_{\text{SecRep}}$ | Uptime (%) |
|---------------|--------------------------------------------------|-------|-------|--------------------|--------------------|---------------------|------------|
| 61219 – 61249 | -17101.85                                        | 0.02  | 0.36  | 4.54               | 0.69               | 1.7                 | 15.4       |

(b) Budget of uncertainties in  $1 \times 10^{-16}$

|                    |                                                           |      |
|--------------------|-----------------------------------------------------------|------|
| $u_A$              | Yb statistics                                             | 0.02 |
|                    | <b><math>u_A</math> total</b>                             | 0.02 |
| $u_B$              | Yb systematics                                            | 0.14 |
|                    | Gravitational redshift <sup>(1)</sup>                     | 0.33 |
|                    | <b><math>u_B</math> total</b>                             | 0.36 |
| $u_{A/\text{Lab}}$ | Yb-HM comparison                                          | 1.01 |
|                    | HM drift <sup>(2)</sup>                                   | 0.06 |
|                    | Dead time in HM – Yb <sup>(3)</sup>                       | 4.42 |
|                    | <b><math>u_{A/\text{Lab}}</math> total</b>                | 4.54 |
| $u_{B/\text{Lab}}$ | Frequency comb <sup>(4)</sup>                             | 0.69 |
|                    | <b><math>u_{B/\text{Lab}}</math> total <sup>(5)</sup></b> | 0.69 |

(1) The height of Yb atoms in the optical lattice of KRISS-Yb1 from the conventionally adopted geoid

potential ( $62\,636\,856.0\text{ m}^2/\text{s}^2$ ) was measured to be  $75.15(4)\text{ m}$ . The height from the earth ellipsoid (WGS84) [3] was measured by a GPS antenna and orthometric height leveling. It is expected that the tidal effect will be averaged out to be small because of the long duration of the measurement campaign. However, because KRISS-Yb1 is operated only intermittently, the average out of the tidal effect might not be sufficient in  $\sim 30$  day measurement. Thus, we conservatively took typical variations from tides to be  $0.3\text{ m}$  [4]. Accordingly, the gravitational shift was conservatively estimated to be  $81.93(33)\times 10^{-16}$ , considering the tidal effect.

- (2) The frequency drift of the hydrogen maser was obtained using the measured data relative to KRISS-Yb1 for 30 days (MJD 61219-61249) including the evaluation period.
- (3) The frequency uncertainty due to the dead-time in HM-Yb comparison was estimated following the procedure in [5, 8]. The noise of HM1405624 was estimated as the square sum of white phase noise  $1.0\times 10^{-13}\text{ (}\tau/\text{s)}^{-1}$ , white frequency noise  $5.0\times 10^{-14}\text{ (}\tau/\text{s)}^{-1/2}$ , flicker frequency noise  $5.0\times 10^{-16}$ , and random walk frequency noise  $1.0\times 10^{-18}\text{ (}\tau/\text{s)}^{1/2}$  as shown Fig. 1. The frequency instability of HM1405624 was deduced by the measurements by three-cornered hat method using two other H-masers, by the Yb optical lattice clock (KRISS-Yb1), and by TT for six months (from Nov. 2025 to Apr. 2026).

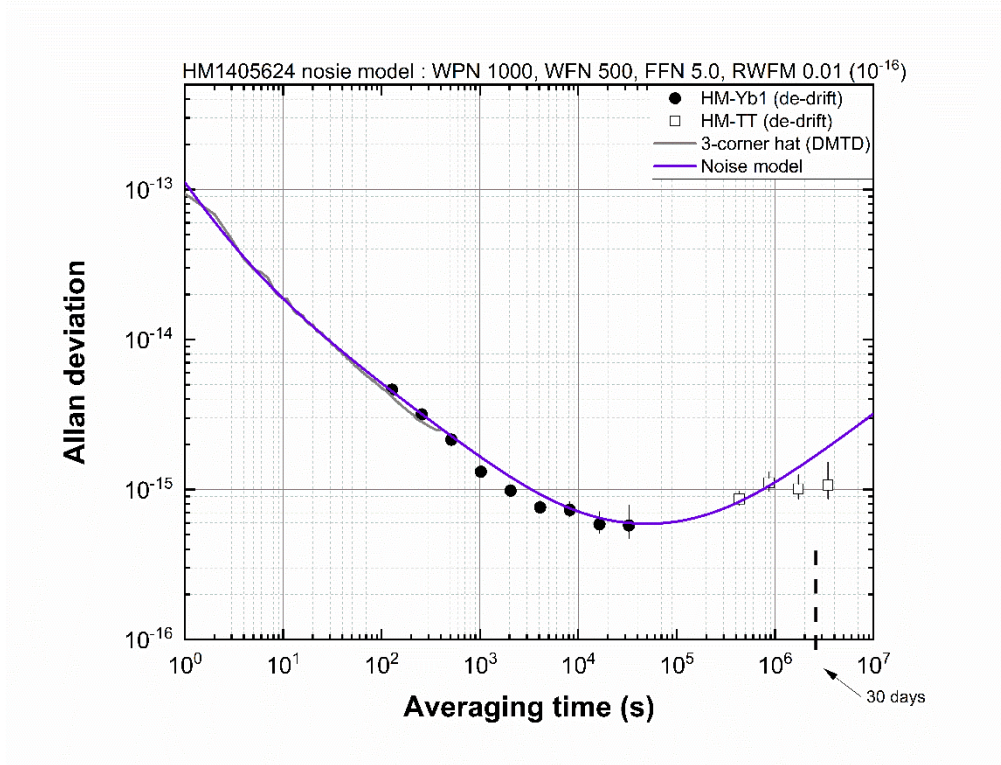


Figure 1. Frequency instability of the hydrogen maser (HM1405624)

- (4) The systematic uncertainty of the frequency conversion by the optical frequency comb from RF to optical frequency was estimated by comparing the simultaneous measurement of the 1156 nm clock laser by two similar optical frequency combs. The weighted mean of the measurement values of the difference between the two comb systems was  $6.6(6.9)\times 10^{-17}$ . There was no difference between the two comb measurements within the uncertainty. The uncertainty was statistically limited despite long total measurement time because the combs were referenced to a hydrogen maser.
- (5)  $u_B/\text{Lab}$  caused by the cables distributing the hydrogen maser signal was ignored. The HM reference signal was located in the same building as KRISS-Yb1 and most part of the cable path was in the temperature-stable laboratory. Also, we used cables with low sensitivity to the temperature variation. Thus, it is expected that the systematic uncertainty due to the cable is negligible. We evaluated the effect from the cable by measuring the frequency difference between the original HM reference signal and the round-

tripped signal (using the two cables of same type along the same path between KRISS-Yb1 and HM). The measured frequency difference is less than the statistical uncertainty, which is given by the Allan deviation value of  $2.5 \times 10^{-18}$  at 100 000 s. There was no bump for the diurnal thermal cycle.

## 2. KRISS-Yb1 operation

The uncertainty budget for KRISS-Yb1 for the reported period is given below [2]

| Effect                              | Relative shift ( $\times 10^{-17}$ ) | Relative Uncertainty ( $\times 10^{-17}$ ) |
|-------------------------------------|--------------------------------------|--------------------------------------------|
| Density shift                       | -0.35                                | 0.30                                       |
| Lattice Stark shift                 | -0.72                                | 0.47                                       |
| Quadratic Zeeman shift              | -6.64                                | 0.13                                       |
| Blackbody radiation                 | -236.39                              | 0.54                                       |
| DC Stark shift <sup>(6)</sup>       | 0.0                                  | 1.00                                       |
| Background gas shift <sup>(7)</sup> | -1.81                                | 0.34                                       |
| Probe light shift                   | 0.06                                 | 0.03                                       |
| Servo error                         | 0.00                                 | 0.27                                       |
| Line pulling                        | 0.00                                 | 0.06                                       |
| AOM chirp                           | 0.00                                 | 0.31                                       |
| <b>Yb Total</b>                     | <b>-245.14</b>                       | <b>1.36</b>                                |

(6) The evaluation of the DC Stark shift would be clearest if we could apply external DC electric field to the trapped Yb atoms. However, this was not possible because our vacuum chamber is made of a solid lump of stainless steel with 9 long and narrow bores (the largest bore diameter is about 35 mm), the external electric fields are attenuated by a factor of  $> 10^4$ , which was estimated by a numerical simulation. However, the advantage of this Faraday shield is that the Yb atoms are insensitive to the electric fields outside the vacuum chamber including the DC electric field due to the charge on dielectric material outside the chamber. The only dielectric material inside the vacuum chamber are two lenses, which are 34.6 mm away from atoms. In our 2017 paper [6], we estimated the electric charges on these lenses would decay with time constant of about 90 days. Since the vacuum installation was done more than 6 years ago ( $\sim 24$  times of the decay time constant), it is estimated the possible Stark shift from the remaining charges is much below  $1 \times 10^{-17}$  if there was no further accumulation of charges. We conservatively took the uncertainty of the DC Stark shift to be  $1 \times 10^{-17}$  as we didn't measure the DC Stark shift directly. Initially, before the experiment for our 2017 paper, we irradiated UV light into the vacuum chamber through the lens pair to make it certain that there was no charge on the lenses. We cannot completely exclude the possibility of charges could newly accumulate. Because we do not have another Yb clock running now, it is not possible to observe the effect of the newly accumulated charges if the charge amount is small. We can estimate the upper limit of the possible DC Stark shift by investigating the Yb frequency with uptime, assuming that the laser exposure is the dominant reason for the generation of the charges. If we assume the new charges

happen to be added on the lenses (by the photoelectric effect or the photo-ionization, for example), the steady-state charge on the lenses will be proportional to the rate of the new charge deposition and the charge decay constant. It is expected that the new charge deposition rate should be proportional to the uptime of the optical clock operation. Accordingly, the electric field due to the new charge will be proportional to the clock uptime, and the DC Stark shift will be proportional to the square of the uptime. In August 2021, the operation time of the optical clock was 40%, which includes the experiments for the absolute frequency measurement and also for the systematic evaluation. The absolute frequency in August 2021 was different from the CIPM recommended value by  $2.5 \times 10^{-16}$  with the uncertainty of  $5.3 \times 10^{-16}$ . For the total measurement campaign for our 2021 paper [2], the average uptime was 5.7% and the  $f(\text{Yb/SI})$  was  $2.9 \times 10^{-16}$  from the CIPM recommended value with the uncertainty of  $2.6 \times 10^{-16}$ . When we compare the two results, there is no frequency difference within the uncertainties of the two measurements. The uptime ratio between the two measurements is 7.0 and there should be 49 times larger DC Stark shift in the 2021 August measurement, but the shift was not noticeable. Thus, it can be inferred that the upper limit of the DC Stark shift in August 2021 is given by the frequency measurement uncertainty of  $5.3 \times 10^{-16}$ , and the upper limit of the DC Stark shift for the total measurement campaign will be 49 times lower ( $1.1 \times 10^{-17}$ ). Thus, it can be concluded that the estimated uncertainty of the DC Stark shift is not underestimated even in the worst case.

- (7) The background gas was dominated by  $\text{H}_2$ , which was determined by a residual gas analyzer. This shift was known to be proportional to the trap loss rate. We took the coefficient to be  $1.6(3) \times 10^{-17}$  s from the INRIM work [7], in which the uncertainty includes possible contributions from Yb-Yb collisions as well as Yb- $\text{H}_2$  collisions.

### 3. Frequency measurement

The optical lattice clock was operated for 399,853.0 s (15.4% of the total evaluation period). We compared the frequency of KRISS-Yb1 with the frequency of the H maser (BIPM code 1405624) during the period MJD 61219 – 61249 using an optical frequency comb and a multi-channel dual-mixer time difference (DMTD) measurement system.

The mean fractional frequency deviation of the hydrogen maser over the evaluation period was obtained by the extrapolation of the frequency measurement data to the midpoint of the evaluation period considering the hydrogen maser frequency drift. The frequency drift of the hydrogen maser was obtained using the measured data relative to KRISS-Yb1 for 30 days (MJD 61219-61249) including the evaluation period. The data points and the distribution of the uptimes of KRISS-Yb1 are shown in Fig.2. The dead time uncertainty due to the intermittent measurement was estimated using the experimentally determined noise model of the hydrogen maser; white phase noise  $1.0 \times 10^{-13} (\tau/\text{s})^{-1}$ , white frequency noise  $5.0 \times 10^{-14} (\tau/\text{s})^{-1/2}$ , flicker frequency noise  $5.0 \times 10^{-16}$ , and random walk frequency noise  $1.0 \times 10^{-18} (\tau/\text{s})^{1/2}$ . The uncertainty  $u_A$  is the uncertainty originating from the instability of KRISS-Yb1, which was evaluated by interleaved measurements, shown in Fig.3. The uncertainty  $u_B$  is the sum of the Yb systematic uncertainty for the reported period and the uncertainty of the gravitational redshift relative to the conventional geoid potential  $W_0 = 62\,636\,856.0 \text{ m}^2\text{s}^{-2}$ . The uncertainty  $u_{A/\text{Lab}}$  is given by

the square root of the square sum of the statistical uncertainties from the frequency comb measurement, the hydrogen maser drift compensation and the dead-time of the Yb clock measurement. The uncertainty  $u_{B/Lab}$  is the systematic uncertainty in the comb link between the HM microwave signal and the Yb optical frequency signal, and was evaluated by comparing the simultaneous measurement of the 1156 nm clock laser by two similar optical frequency combs.

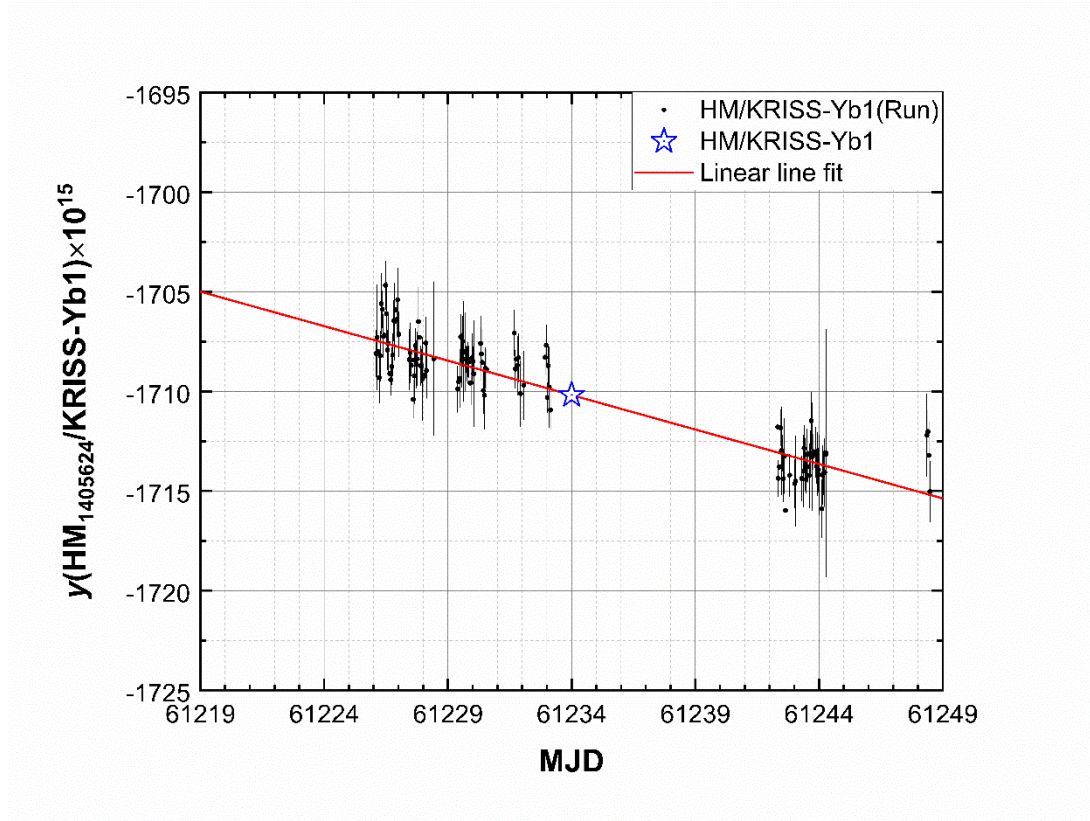


Figure 2. The black points are averaged data of  $y(HM_{1405624}/KRISS-Yb1)$  over around 3,600 s or less operation time with each uncertainty. The blue star indicates the determined value of  $y(HM_{1405624}/KRISS-Yb1)$ . The red line is the linear fit (drift rate :  $-0.346 \times 10^{-15}/d$ ) using data from MJD 61219 to MJD 61249.



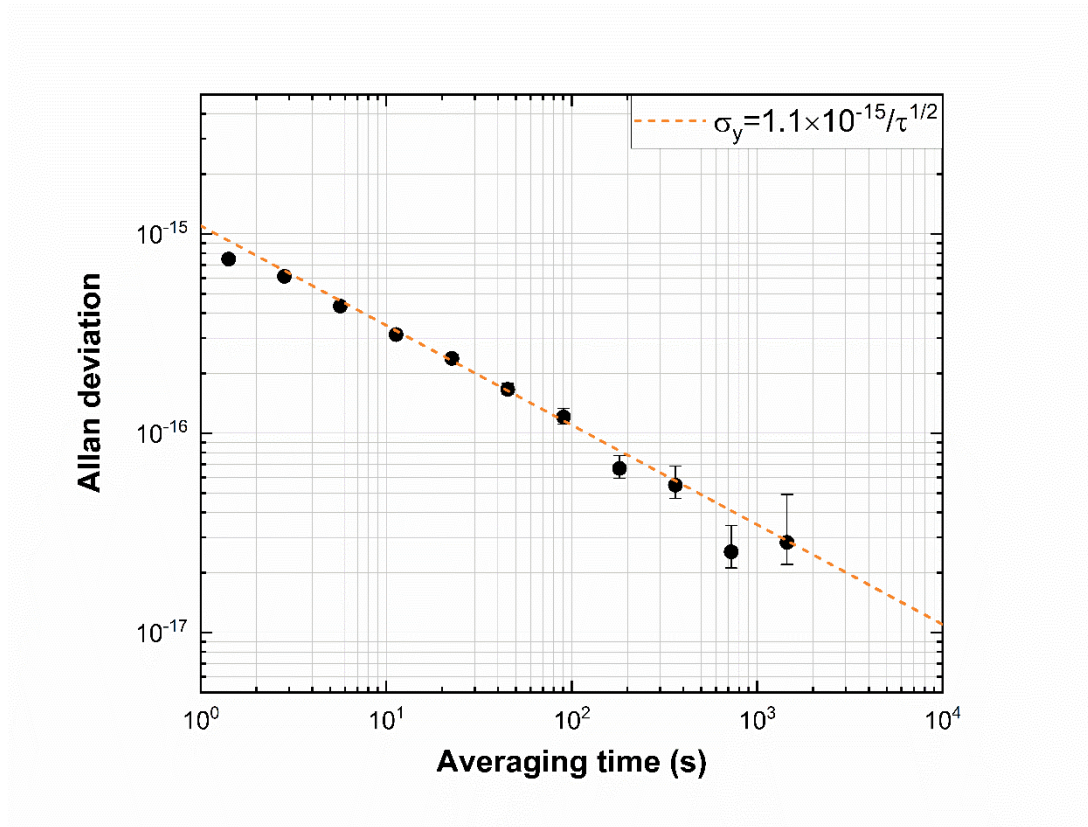


Figure 3. Stability of KRISS-Yb1 in terms of overlapping Allan deviation of the frequency difference between the two interleaved measurements.

#### ▣ Remarks on the change history of the report

- (1) The first report by KRISS-Yb1 was for the period MJD 58864 – 58874 (Jan. 16, 2020 – Jan. 26, 2020) evaluating the frequency of HM1405628.
- (2) The hydrogen maser, which was evaluated by KRISS-Yb1, was changed to HM1405626 from MJD 59029 (Jun. 29, 2020) to MJD 59579 (Dec. 31, 2021).
- (3) The hydrogen maser, which was evaluated by KRISS-Yb1, was changed to HM1405628 from MJD 59579 (Dec. 31, 2021) to MJD 60444 (May. 14, 2024).
- (4) The hydrogen maser, which was evaluated by KRISS-Yb1, was changed to HM1405626 from MJD 60789 (Apr. 24, 2025) to MJD 60824 (May. 29, 2025).
- (5) The hydrogen maser, which is to be evaluated by KRISS-Yb1, has been changed to HM1405624 since MJD 60824 (May. 29, 2025).

- (6) The KRISS-Yb1 absolute frequency has been assumed to be the 2021 BIPM-recommended value (518,295,836,590,863.63 Hz) since MJD 59669 (Mar. 31, 2022).
- (7) The height of Yb atoms in the optical lattice of KRISS-Yb1 from the conventionally adopted geoid potential ( $62\,636\,856.0\text{ m}^2/\text{s}^2$ ) was updated from 75.07(9) m to 75.15(4) m by the new height measurement [3]. The two height measurements agree with each other within the uncertainty. Accordingly, the gravitational shift was modified from  $81.9(3)\times 10^{-16}$  to  $81.93(33)\times 10^{-16}$  at MJD 60339.
- (8) Under the updated cooling conditions, the density shift coefficient has been re-evaluated. The resulting linear coefficient is determined to be  $-1.538(620)\text{ }\mu\text{Hz/Atom}$ .

## References

- [1] “Recommended values of standard frequencies for applications including the practical realization of the metre and secondary representations of the definition of the second,” BIPM publication, approved by CCTF September 2025, [https://www.bipm.org/documents/20126/288516347/171Yb\\_518THz\\_2025/73007ecc-49f5-4d1d-d8ee-6793a4748598](https://www.bipm.org/documents/20126/288516347/171Yb_518THz_2025/73007ecc-49f5-4d1d-d8ee-6793a4748598)
- [2] Huidong Kim et al, “Absolute frequency measurement of the  $^{171}\text{Yb}$  optical lattice clock at KRISS using TAI for over a year”, *Metrologia*, 58, 055007 (2021)
- [3] Jisun Lee et al, “Evaluation of the relativistic redshift in frequency standards at KRISS”, *Metrologia*, 61, 015008 (2024)
- [4] C. Voigt et al, “Time-variable gravity potential components for optical clock comparisons and the definition of international time scales”, *Metrologia*, 53, 1365 (2016)
- [5] D.-H. Yu et al, “Uncertainty of a frequency comparison with distributed dead time and measurement interval offset”, *Metrologia*, 44, 91 (2007)
- [6] Huidong Kim et al, “Improved absolute frequency measurement of the  $^{171}\text{Yb}$  optical lattice clock at KRISS relative to the SI second”, *Japan. J. Appl. Phys.* 56, 050302 (2017)
- [7] M. Pizzocaro et al, “Absolute frequency measurement of the  $^1\text{S}_0\text{--}^3\text{P}_0$  transition of  $^{171}\text{Yb}$  with a link to Int. Atomic Time”, *Metrologia* 57, 035007 (2020)
- [8] H. Hachisu et al, “Intermittent optical frequency measurements to reduce the dead time

uncertainty of frequency link”, Japan. J. Appl. Phys. 54, 112401 (2015)