

Frequency evaluation of UTC(NPL) by NPL-Sr1 for the period MJD 57904 to MJD 57919

National Physical Laboratory

March 20, 2023

The secondary frequency standard NPL-Sr1 and an optical frequency comb were used to evaluate the frequency of UTC(NPL) over a period of 15 days from MJD 57904 to MJD 57919 (31st May 2017 – 15th June 2017). The Sr optical lattice clock operation covers 74.0% of the total measurement period. The result of the evaluation is reported in table 1 and is made using the CCTF 2021 recommended frequency value for the $5s^2\ ^1S_0 - 5s5p\ ^3P_0$ unperturbed optical transition in ^{87}Sr : 429 228 004 229 872.99 Hz with a relative standard uncertainty of $u_{\text{Srep}} = 1.9 \times 10^{-16}$ [1].

Period of estimation	$y(\text{UTC(NPL)} - \text{NPL-Sr1}) / 10^{-16}$	$u_A / 10^{-16}$	$u_B / 10^{-16}$	$u_{A/\text{Lab}} / 10^{-16}$	$u_{B/\text{Lab}} / 10^{-16}$	$u_{\text{Srep}} / 10^{-16}$	Uptime
MJD 57904–57919	-2.12	0.020	0.11	1.32	1.12	1.9	74.0%

Table 1: Results of the evaluation of UTC(NPL) by NPL-Sr1.

1 Measurement configuration

NPL-Sr1 was operated as described in reference [2]. The 698 nm clock laser was pre-stabilized to a local reference cavity and then phase-locked via a fibre-based optical frequency comb to another more stable laser, at either 1064 nm or 934 nm. A feedback loop acting on an acousto-optic modulator (AOM) kept the clock laser frequency in resonance with the ^{87}Sr clock transition. The optical frequency comb was referenced to UTC(NPL), and the frequency ratio between the ^{87}Sr clock transition and UTC(NPL) was calculated from the comb measurements of the 698 nm ultrastable laser and the AOM frequency corrections. The reported frequency value is determined as the average of a sawtooth fit to the NPL-Sr1/UTC(NPL) ratio data, which includes frequency steps corresponding to the known times and magnitudes of the maser frequency steers.

2 NPL-Sr1 evaluation

Type A uncertainty

The type A uncertainty u_A is the statistical contribution from the frequency instability of NPL-Sr1. This was estimated based on a white frequency noise component of $2 \times 10^{-15} / \sqrt{\tau}$, extrapolated to the duration of the evaluation period. This is a conservative upper bound, based on measurements against another optical lattice clock, performed over an optical fibre network [3].

Systematic effect	Correction / 10^{-18}	Uncertainty / 10^{-18}
BBR chamber	4854.2	7.0
BBR oven	0.5	0.5
Quadratic Zeeman	287.0	3.0
Lattice	-1.6	4.0
Collisions	0.9	3.8
Background gas	3.8	3.8
DC Stark	0.016	0.016
Probe Stark	1.0	0.4
Servo Error	0.0	2.0
Total correction	5145.8	10.4
Gravitational redshift	-1215.0	2.7
Total including gravitational redshift	3930.8	10.7

Table 2: Uncertainty budget of the NPL-Sr1 lattice clock for this evaluation period. Reported uncertainties correspond to 68% confidence intervals.

Type B uncertainty

The type B uncertainty u_B is the sum in quadrature of the systematic uncertainty of NPL-Sr1 and the uncertainty of the gravitational redshift relative to the conventionally adopted reference potential $W_0 = 62\,636\,856.0 \text{ m}^2\text{s}^{-2}$. The uncertainty evaluation of NPL-Sr1 is described in [2], and the systematic frequency corrections and uncertainty budget for the period of this report are given in table 2. The geopotential value for NPL-Sr1 is taken from [4].

Changes to the uncertainty evaluation presented in reference [2] are described below. We also note that subsequent to this evaluation, an updated dynamic correction coefficient for blackbody radiation was reported in reference [5]. This would increase the total BBR correction by approximately 4×10^{-18} for our operational conditions at close to 300 K, but we have not revised the uncertainty budget here to account for this.

Background gas

For this evaluation we use an updated coefficient for the background gas collisional shift of $(-3.0 \pm 0.3) \times 10^{-17}/\tau$, where τ is the $1/e$ vacuum-limited trap lifetime [6]. Assuming hydrogen is the dominant gas in our system we arrive at a shift of -3.8×10^{-18} based on lattice trapped lifetime measurements of 8 s. However, since the gas composition is only assumed, and the lifetime measurement may be reduced by parametric heating in the lattice trap, we assign an uncertainty equal to the shift.

3 Frequency comparison

Type A uncertainty

The uncertainty $u_{A/\text{Lab}}$ arises from the dead time in the comparison between UTC(NPL) and NPL-Sr1, and includes both a deterministic correction due to maser drift and a stochastic contribution (table 3).

Contribution	Uncertainty / 10^{-18}
$u_{\text{A/Lab}}$ [Deterministic]	24
$u_{\text{A/Lab}}$ [Stochastic]	130
$u_{\text{A/Lab}}$ [Total]	132

Table 3: A breakdown of the uncertainties included in $u_{\text{A/Lab}}$.

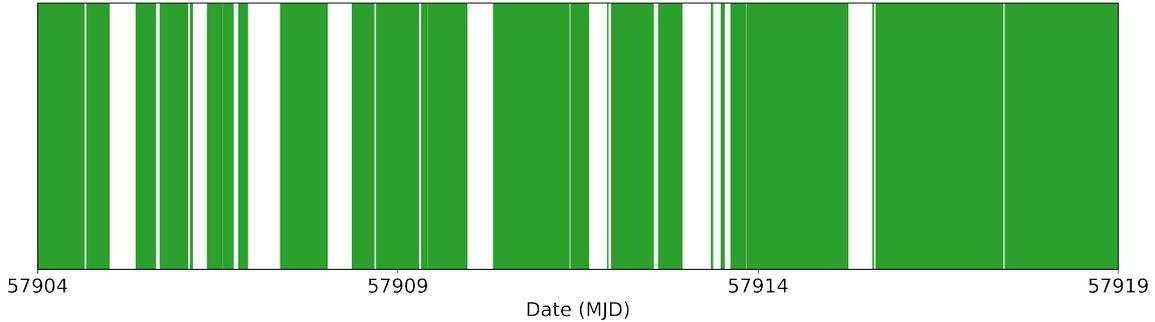


Figure 1: Uptime of NPL-Sr1 over the evaluation period (green regions).

The stochastic contribution was estimated by a method described in reference [7]. This involves a Monte-Carlo approach where the frequency noise of UTC(NPL) is simulated and a value calculated for the offset between the mean frequency during the uptime periods and the mean frequency during the whole evaluation period. The simulation was repeated 1000 times, with the standard deviation of the offsets providing an estimate for the frequency uncertainty arising from the dead times in the operation of NPL-Sr1. The maser noise model used comprised white phase noise of $4 \times 10^{-13}/\tau$, white frequency noise of $12 \times 10^{-14}/\sqrt{\tau}$, and a flicker frequency floor of 0.8×10^{-15} . These values were derived from measurements of UTC(NPL) by NPL-Sr1.

For this evaluation period, NPL-Sr1 had an uptime of 74%, distributed as shown in figure 1.

Type B uncertainty

The uncertainty $u_{\text{B/Lab}}$ is dominated by the distribution of the 10 MHz signal from the maser generating UTC(NPL) to the frequency comb laboratory, and the subsequent synthesis in that laboratory of an 8 GHz signal against which the repetition rate of the frequency comb was measured. Potential phase fluctuations were monitored using a loop-back comparison as described in reference [2], and their contribution to the uncertainty estimated from the instability of these fluctuations over the evaluation period. (Note that this is slightly different to the uncertainty reported in [2], which used data from the whole month.)

References

- [1] Consultative Committee for Time and Frequency (CCTF), “[Recommendation PSFS-2 from the 22nd meeting \(session II – online\)](#),” (2022).
- [2] R. Hobson, W. Bowden, A. Vianello, A. Silva, C. F. A. Baynham, H. S. Margolis, P. E. G.

- Baird, P. Gill, and I. R. Hill, “A strontium optical lattice clock with 1×10^{-17} uncertainty and measurement of its absolute frequency,” *Metrologia* **57**, 065026 (2020).
- [3] P. Delva, J. Lodewyck, S. Bilicki, E. Bookjans, G. Vallet, R. Le Targat, P.-E. Pottie, C. Guerlin, F. Meynadier, C. Le Poncin-Lafitte, O. Lopez, A. Amy-Klein, W.-K. Lee, N. Quintin, C. Lisdat, A. Al-Masoudi, S. Dörscher, C. Grebing, G. Grosche, A. Kuhl, S. Raupach, U. Sterr, I. R. Hill, R. Hobson, W. Bowden, J. Kronjäger, G. Marra, A. Rolland, F. N. Baynes, H. S. Margolis, and P. Gill, “Test of special relativity using a fiber network of optical clocks,” *Phys. Rev. Lett.* **118**, 221102 (2017).
- [4] F. Riedel, A. Al-Masoudi, E. Benkler, S. Dörscher, V. Gerginov, C. Grebing, S. Häfner, N. Hunte-mann, B. Lipphardt, C. Lisdat, E. Peik, D. Piester, C. Sanner, C. Tamm, S. Weyers, H. Denker, L. Timmen, C. Voigt, D. Calonico, G. Cerretto, G. A. Costanzo, F. Levi, I. Sesia, J. Achkar, J. Guéna, M. Abgrall, D. Rovera, B. Chupin, C. Shi, S. Bilicki, E. Bookjans, J. Lodewyck, R. L. Targat, P. Delva, S. Bize, F. N. Baynes, C. F. A. Baynham, W. Bowden, P. Gill, R. M. Godun, I. R. Hill, R. Hobson, J. M. Jones, S. A. King, P. B. R. Nisbet-Jones, A. Rolland, S. L. Shemar, P. B. Whibberley, and H. S. Margolis, “Direct comparisons of European primary and secondary frequency standards via satellite techniques,” *Metrologia* **57**, 045005 (2020).
- [5] C. Lisdat, S. Dörscher, I. Nosske, and U. Sterr, “Blackbody radiation shift in strontium lattice clocks revisited,” *Phys. Rev. Research* **3**, L042036 (2021).
- [6] B. X. R. Alves, Y. Foucault, G. Vallet, and J. Lodewyck, “Background Gas Collision Frequency Shift on Lattice-Trapped Strontium Atoms,” in *2019 Joint Conference of the IEEE International Frequency Control Symposium and European Frequency and Time Forum (EFTF/IFC)* (IEEE, Orlando, FL, USA, 2019) pp. 1–2.
- [7] D.-H. Yu, M. Weiss, and T. E. Parker, “Uncertainty of a frequency comparison with distributed dead time and measurement interval offset,” *Metrologia* **44**, 91 (2007).