

**FREQUENCY COMPARISON (H_MASER 140 0890) - (LNE-SYRTE-FO2)
For the period MJD 55804 to MJD 55834**

The primary frequency standard LNE-SYRTE-FO2 has been compared to the hydrogen Maser 140 0890 of the laboratory, during a measurement campaign between MJD 55804 and 55834 (31st August 2011 – 30th September 2011). The fountain operation covers ~ 82 % of the total measurement duration. The collected data have been separated in 2 intervals of 15 days duration to better take into account a variation of the maser's frequency drift.

The mean frequency difference at the middle date each period is given in the following table:

Period (MJD)	Date of the estimation	y(HMaser _{140 0890} – FO2)	u_B	u_A	$u_{link / maser}$
55804 – 55819	55811.5	-666.3	2.7	2	1.7
55819 – 55834	55826.5	-695.0	2.7	3	1.0

Table 1: Results of the comparison in 1×10^{-16} .

The FO2 fountain was operated in the same mode during all the period: the interrogating signal synthesis is based on the down conversion to 9.192 GHz of a 11.98 GHz signal provided by a cryogenic oscillator phase locked to the maser 140 0890. It uses a synthesizer to lock the microwave signal on the atomic resonance. The frequency difference between this maser and the fountain is deduced from the average correction applied to the synthesizer.

Average value and statistical uncertainty

This paragraph describes the calculation of the average frequency of HMaser_{140 0890}-FO2. The details of the calculation are given in figure 1 and 2:

The frequency data averaged over 0.2 day are plotted on the upper graph (blue points) together with a linear unweighted fit (red line).

The parameters of the fit $y=a + b(x-x_middle_date)$ are respectively for the 2 segments:

Period (MJD)	a	b
55804 – 55819	$(-666.3 \pm 1.3) \cdot 10^{-16}$	$(-5.1 \pm 0.3) \cdot 10^{-16}/\text{day}$
55819 – 55839	$(-695.0 \pm 1.1) \cdot 10^{-16}$	$(+1.1 \pm 0.3) \cdot 10^{-16}/\text{day}$

Table 2: coefficients of the linear fit of HMaser_{140 0890}-FO2

These coefficients are used to remove the drift (data plotted in the graph in the middle, red points) and to calculate the average value at middle date, given in table 1. The lower graph gives the variance of the frequency residuals. We estimate a conservative statistical uncertainty u_A of 2×10^{-16} and 3×10^{-16} for the two segments respectively.

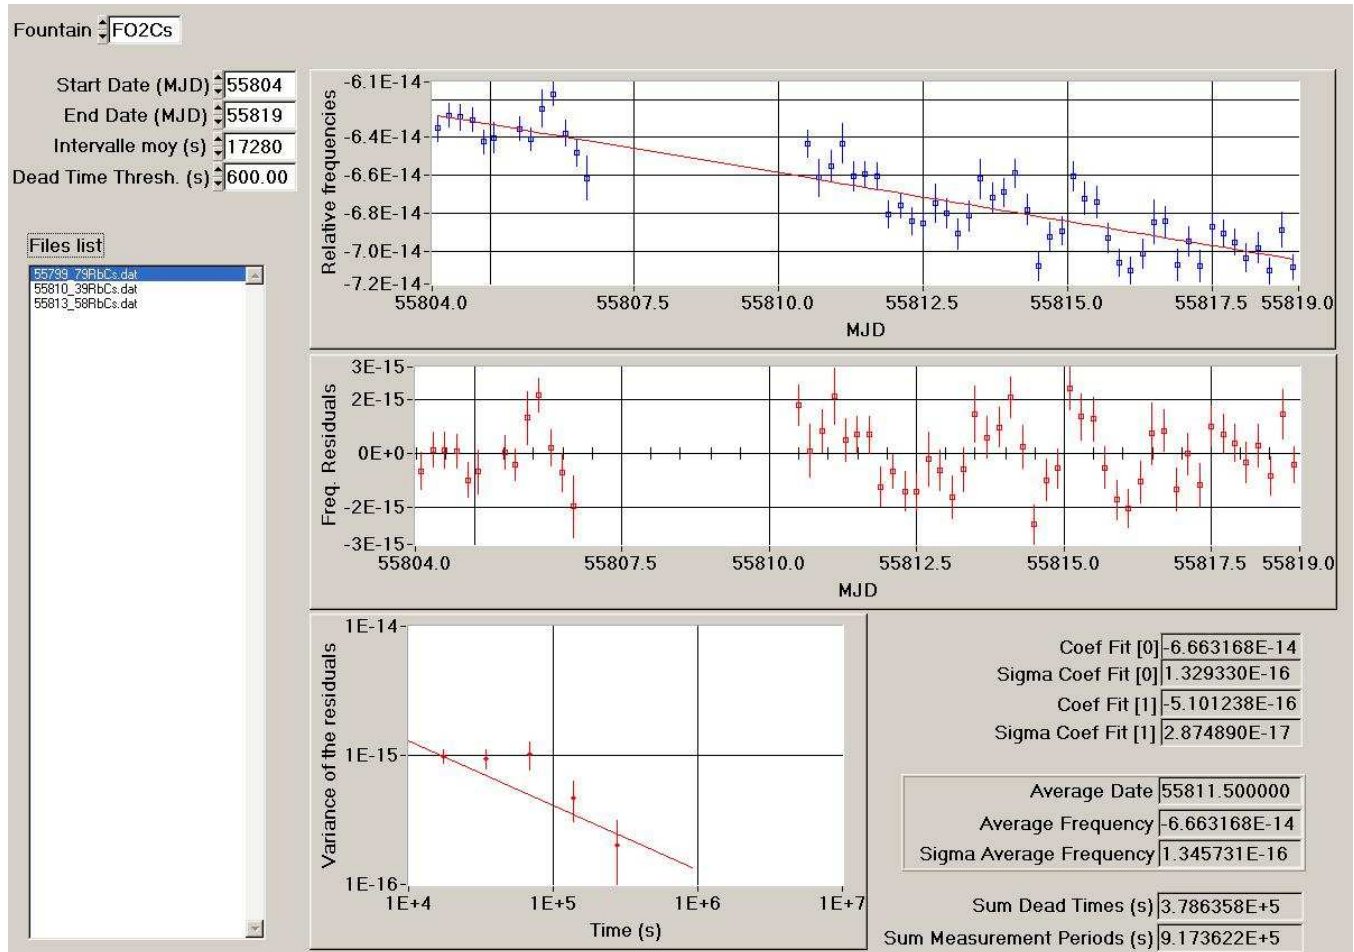


Figure 1: Processing of the data $HMaser_{140\ 0890-FO2}$ for the period MJD 55804-55819

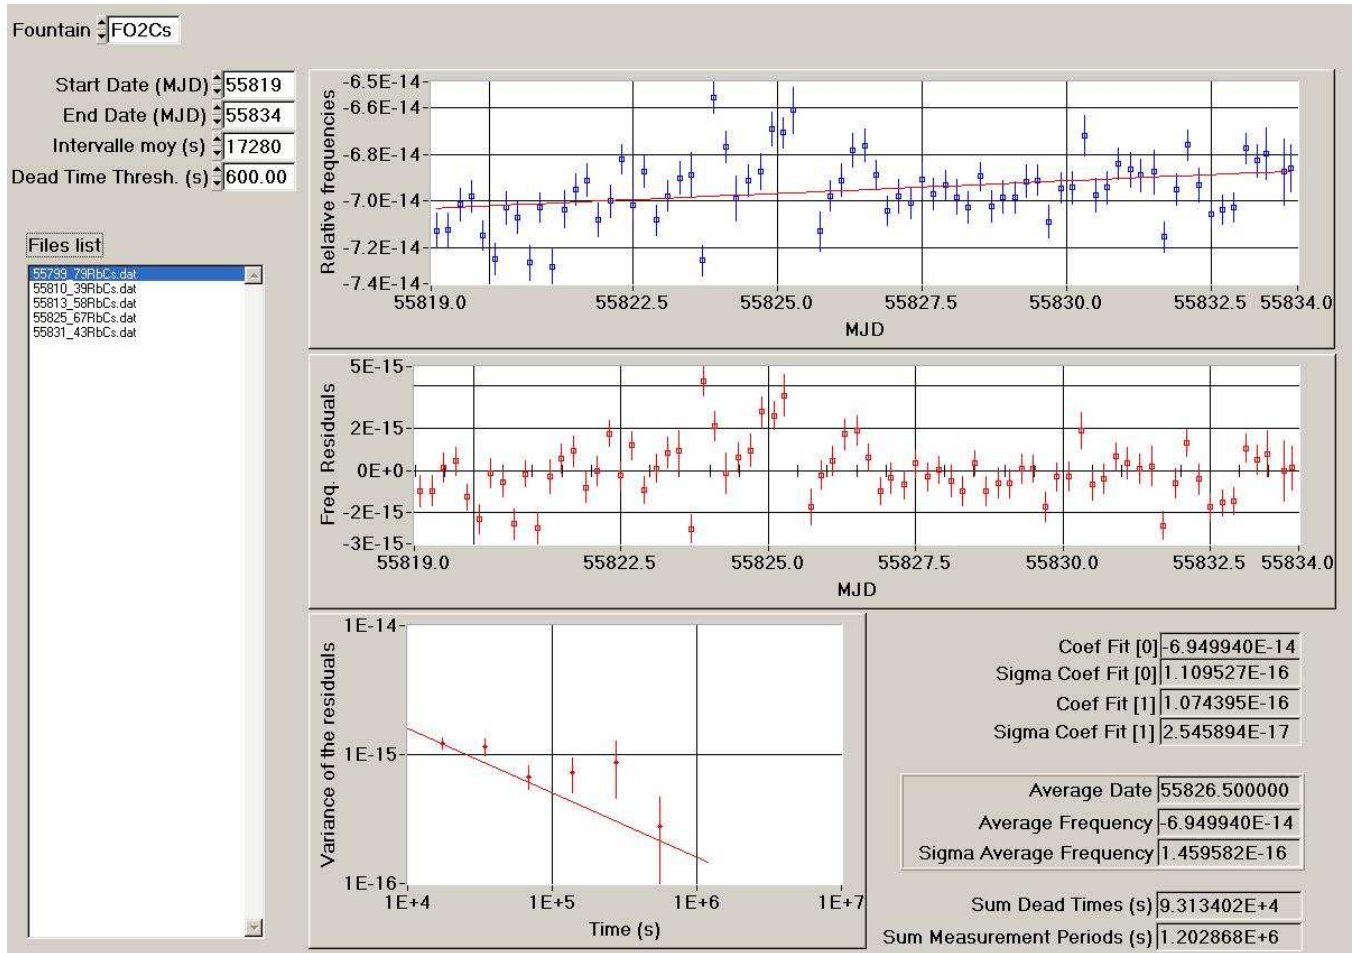


Figure 2: Processing of the data $HMaser_{140\ 0890-FO2}$ for the period MJD 55819-55834

We verified the result by applying a second method. We calculated the accumulated phase by integrating the data points, assuming a linear frequency drift during each segment, and during the dead times of the fountain operation. The average frequency is then obtained by dividing the total accumulated phase by the calibration period duration. The processing has been performed with segments of 0.01, 0.1 and 1 day durations. The differences between the results and the value given in table 1 are in agreement within 2.0×10^{-16} and 1.0×10^{-16} for the two segments respectively, which is consistent with the estimations of the statistical uncertainty u_A and the uncertainty due to the link.

Accuracy

The frequency is corrected from the quadratic Zeeman, the Black Body radiation, the cold collisions and cavity pulling, and the red shift effects. Here the uncertainty in the cold collisions correction accounts for both a statistical uncertainty and a systematic uncertainty taken as 0.5% of the correction for high density measurements. The following table summarizes the budget of systematic effects and their associated uncertainties. The accuracy is the quadratic sum of all the systematic uncertainties.

	Correction (10^{-16})	Uncertainty (10^{-16})
Quadratic Zeeman effect	-1916.6	0.3
Black body radiation	168.2	0.6
Cold collisions and cavity pulling	58.65	1.5
First order Doppler	-0.75	0.93
Microwave spectral purity&leakage	0	<0.5
Ramsey & Rabi pulling	0	< 0.1
Microwave lensing	0	< 1.4
Second order Doppler effect	0	< 0.1
Background gas collisions	0	<1.0
Total	-1690.5	2.53
Red shift	- 65.4	1.0
Total with red shift	-1755.9	2.72

Table 2: Budget of systematic effects and uncertainties for SYRTE-FO2 fountain for the MJD 55804– 55834 period

$$\boxed{u_B = 2.7 \times 10^{-16}}$$

Uncertainty of the link

The uncertainty of the link is the quadratic sum of 2 terms:

-A possible effect of phase fluctuations introduced by the cables that connect the primary standard to the Maser. It is estimated to be 10^{-16} .

-The uncertainty due to the dead times of the frequency comparison.

To estimate this contribution, we use the comparison between the reference Maser and Maser 140 0816.

We calculate the time deviation of the normalized phase differences with the linear frequency drift removed. The uncertainty is given by:

$$\sigma_{y_{Dead\ Time}} = \frac{\sqrt{\sum_i \sigma_{x_i}^2}}{T}$$

where σ_{x_i} are the extrapolated TVar for each dead times. We applied the method to the dead times longer than 600 s and obtained stability degradation of 1.4×10^{-16} and 0.2×10^{-16} for the two segments respectively.