

GNSS CALIBRATION REPORT

G1G2_ 1018-2021

Prepared by: Carmen Vélez (ROA)

Approved by: Héctor Esteban (ROA)

Authorized by: BIPM

Project: EURAMET_ROA_G1G2

Code: 1018-2021

Version: 1.0

Date: 09/12/2021

TABLE OF CONTENTS

1. INTRODUCTION	4
1.1. SCOPE OF THE DOCUMENT	4
1.2. DOCUMENT STRUCTURE	4
1.3. DOCUMENTS	5
1.4. ACRONYMS AND ABBREVIATIONS	5
2. PARTICIPANTS AND SCHEDULE	7
3. THE ROA TRAVELING EQUIPMENT	8
4. CALIBRATION PROCEDURE.....	9
5. DATA PROCESSING.....	10
6. UNCERTAINTY ESTIMATION.....	12
7. FINAL RESULTS	13
8. ANNEX-A.....	14
8.1. CALIBRATION INFORMATION SHEET AT ROA.....	14
8.2. CALIBRATION INFORMATION SHEET AT NPL.....	16
9. ANNEX-B: CCD AT EACH LAB.....	24

LIST OF TABLES AND FIGURES

Table 1-1: List of Acronyms and Abbreviations.....	5
Table 2-1: List of participants.	7
Table 2-2: Schedule of the campaign and involved receivers.	7
Table 5-1: Initial delays (in ns) of receivers at start of calibration.	10
Table 6-1: Uncertainty contributions for the calibration of receiver delays	12
Table 7-1: GPS calibration results, all values in ns.....	13
Table 7-2: Galileo calibration results, all values in ns.	13
Figure 9-1: Before the calibration trip (GPS).....	24
Figure 9-2: Before the calibration trip (Galileo)	24
Figure 9-3: After the calibration trip (GPS)	25
Figure 9-4: After the calibration trip (Galileo)	25
Figure 9-5: GPS CCD at NPL	26
Figure 9-6: Galileo CCD at NPL	28

1. INTRODUCTION

1.1. SCOPE OF THE DOCUMENT

In 2014, as a result of a CCTF recommendation for a collaboration between the BIPM and the RMOs for GNSS equipment calibration, some National Metrology Institutes (NMIs) and Designated Institutes (DIs), were selected to be G1 laboratories, to function as regional nodes for the GPS calibrations. The mission of these Labs, once calibrated by BIPM, was to perform new calibration trips among G2 laboratories, under the responsibility of RMOs.

ROA, as EURAMET G1 laboratory, organized this year, a GPS receiver relative calibration campaign, which took place at NPL(UK).

In this campaign was carried out a differential calibration with closure, where the travelling system served as a transfer between all NPL systems and the reference receiver RO_9. This last was calibrated and reported this year (Cal_Id=1018-2021), being continuously monitored since then.

1.2. DOCUMENT STRUCTURE

The current campaign has been carried out in accordance with ROA calibration procedure and following as much as possible the BIPM guidelines for GNSS calibrations [RD02]. The results will be reported using Cal_Id 1018-2021, and they will provide the visited receivers' internal delays for GPS (C1, P1, P2) and Galileo (E1, E5a) code signals.

Section 1 of this document gives the introduction, the document structure and a document baseline (in terms of applicable and reference documents and used acronyms).

Section 2 reports, the participating laboratories, dates of visits, and GPS receivers involved in this calibration campaign.

Section 3 presents an overview of the travelling equipment specifically prepared for this activity.

Section 4 basically describes the calibration procedure.

Section 5 explains the data processing carried out by our own software and all the necessary tables to get the results.

Section 6 is focused in the uncertainty estimation, in all the terms taken into account for the uncertainty budget.

Section 7 shows the final results, with the new internal delays, as well as all the necessary information to get them.

The report concludes with the Annex-A for each visited receiver, and the Annex-B, which contains all the figures with the common clock differences (CCD).

1.3. DOCUMENTS

REFERENCES	
RD01	BIPM report 1001-2020 V1.2 / 20210712, subject: 2021 Group 1 GNSS calibration trip (Phase 2).
RD02	BIPM guidelines for GNSS calibration, V3.2, 15/02/2016.
RD03	G. Petit, Z. Jiang, P. Moussay, J. White, E. Powers, G. Dudle, P. Uhrich, 2001, Progresses in the calibration of geodetic like GPS receivers for accurate time comparisons, Proc. 15th EFTF, pp. 164-166.
RD04	p. Defraigne, C. Bruyninx, 2001, Time Transfer for TAI using a geodetic receiver, An Example with the Ashtech ZXII-T, GPS Solutions, 5(2), pp. 43-50.
RD05	J. Kouba, P. Heroux, 2002, Precise Point Positioning Using IGS Orbit and Clock Products, GPS Solutions, Vol. 5, No. 2, pp. 12-28.

1.4. ACRONYMS AND ABBREVIATIONS

Table 1-1: List of Acronyms and Abbreviations

Acronym	Definition
BIPM	Bureau International des Poids et Mesures.
CCD	Common Clock Difference.
CCTF	Consultative Committee for Time and Frequency.
CGGTTS	CCTF Generic GNSS Time Transfer Standard.
CCTF	Consultative Committee for Time and Frequency.
DI	Designated Institute.
EURAMET	European Association of National Metrology Institutes.
Galileo	European GNSS
GNSS	Global Navigation Satellite System
GPS	Global Positioning System.
IGS	International GNSS Service.
ITRF	International Terrestrial Reference Frame.
MJD	Modified Julian Date.
NMI	National Metrology Institute.
NRCan	Natural Resources Canada.
PPP	Precise Point Positioning.
RINEX	Receiver Independent Exchange Format.
RMO	Regional Metrology Organization.
ROA	Real Instituto y Observatorio de la Armada, San Fernando, Spain.
TDEV	Time Deviation. Is a measure of time stability based on the modified Allan variance.
TIC	Time Interval Counter.
NPL	National Physical Laboratory.
UTC	Coordinated Universal Time.
UTC(k)	Version of UTC realized at each of the contributing NMIs.

Acronym	Definition
CGGTTS specific acronyms	
CAB DLY	Field present in the CGGTTS header. It is the group delay inside the antenna cable, including both end connectors.
INT DLY	Field present in the CGGTTS header. It is the code- and frequency-dependent combined electric delay of the GNSS signal inside the antenna and the receiver. See also [RD03].
REF DLY	Field present in the CGGTTS header. It is the time offset between the receiver internal clock (or its conventional realization by an external signal) and the local clock at the station. See also [RD03].
REFGPS	Time difference between the reference clock and GPS time, for each satellite at the mid-point of the 13 min track. Receiver delay, cable delay, tropospheric delay and (for one single code) modelled ionospheric delay corrections have been applied.

2. PARTICIPANTS AND SCHEDULE

Participating laboratories, dates and GPS receivers involved in the calibration campaign are summarized in Table 2-1 y Table 2-2. Nevertheless, a complete information related with the receiver set-up and the signal distribution system have been provided by all Labs (see relevant Annex-A).

Table 2-1: List of participants.

Institute	Point of contact	Postal address
ROA	Dr Héctor Esteban Tel +34 956599286 hesteban@roa.es	Real Instituto y Observatorio de la Armada Plaza de las Tres Marinas s/n 11100, San Fernando, Spain
NPL	Dr Peter Whibberley Tel +44 20 8943 6746 peter.whibberley@npl.co.uk	National Physical Laboratory Hampton Road Teddington, Middlesex TW11 0LW, UK

Table 2-2: Schedule of the campaign and involved receivers.

Institute	Status of equipment	Dates of measurements	Receiver type	BIPM code	RINEX code
ROA	Traveling		Septentrio PolaRx5TR		TR
ROA	Group 1 reference	MJD: 59419-59423 24/07/21-28/07/21	Septentrio PolaRx4TR	RO_9	RO_9
NPL	Group 2 reference	MJD: 59499-59504 12/10/21-17/10/21	DICOM GTR50	NPL1	NPL1
NPL	Group 2 reference	MJD: 59499-59504 12/10/21-17/10/21	MESIT GTR51	NPL2	NPL2
NPL	Group 2 reference	MJD: 59499-59504 12/10/21-17/10/21	Septentrio PolaRx5TR	NPL3	NPL3
NPL	Group 2 reference	MJD: 59499-59504 12/10/21-17/10/21	MESIT GTR51	NPL4	GAL1
ROA	Group 1 reference	MJD: 59540-59546 22/11/21-28/11/21	Septentrio PolaRx4TR	RO_9	RO_9

3. THE ROA TRAVELING EQUIPMENT

Traveling equipment consists of one shipping box containing the following items:

- 1 PolARx5TR receiver SN: 4701310.
- 1 Portable PC Toshiba Tecra M9 laptop SN: X7052920H.1 Novatel antenna GPS-703-GGG SN:01018146.
- 50 m H155 antenna cable.

As it is shown in the equipment list, only one receiver was used as traveling equipment. We used a direct antenna cable to connect the PolARx5TR and the Novatel antenna.

4. CALIBRATION PROCEDURE

The calibration has been performed based on C1, P3 GPS and E1, E3 CCGTTS Galileo files. Instead using the files automatically generated by each particular receiver, we have generated them from RINEX V.3 observation files, by means of R2CGGTTS software tool V8.3 developed at the Royal Observatory of Belgium [RD04]. This was done to avoid any systematic error induced by the use of a different tropospheric model, and mainly by imprecise antenna positions.

On this latter point, the coordinates of the antenna phase centre at each location have been especially computed for the calibration period from RINEX files by using the NRCan PPP software [RD05], so the time transfer error caused by this factor is nearly negligible.

Basically the calibration consists on the following. From the known delays of the reference receiver (RO_9) and an average of the traveling receiver delays between the start and the end of the campaign, we can obtain INTDLY(C1), INTDLY(P1) and INTDLY(P2) for the receivers in the visited Labs. As the calibration is consisting in building differential pseudo-ranges for each code C1, P1 and P2 between pairs of receivers in common-clock set-up, they can be easily obtained by using the data collected in C1 and also in P3 CCGTTS files:

$$\gamma = (f_1/f_2)^2 = (77/60)^2$$

$$REFGPS(P1) = REFSYS(P3) + MSIO$$

$$REFGPS(P2) = REFGPS(P3) + \gamma \times MSIO$$

where *MSIO* are the measured ionospheric delays.

In a similar way, with $\gamma = (E1/E5a)^2 = (1575.42/1176.45)^2$, INTDLY(E1) and INTDLY(E5a) can be obtained.

5. DATA PROCESSING

For the calculation process we have used a ROA-authored program, in which the common clock differences (CCD) are obtained from the common-view of CGGTTS files. For each location, the coordinates of the antenna have been carefully calculated for the calibration period.

As was stated before, from the known delays of the reference receiver RO_9, it has been obtained the internal delays for each receiver at the visited site. Normally, the antenna cable delay (CABDLY) is maintained without any change, and the reference delay (REFDLY) is normally updated, anyway, any variation with respect to the true values, will be assumed by the INTDLY results.

Table 5-1 summarizes the initial delays of the NPL receivers at the start of calibration. With REF DLY and CAB DLY values, and with INT DLY values set to zero, new CGGTTS files have been generated for these receivers. Tables 5-2 and 5-3 show the raw CCD differences at the visited Lab.

Table 5-1: Initial delays (in ns) of receivers at start of calibration.

BIPM code	INT DLY C1	INT DLY P1	INT DLY P2	INT DLY E1	INT DLY E5a	REF DLY	CAB DLY
NPL1	-37.2	-37.9	-29.0	0.0	0.0	77.2	251.5
NPL2	35.7	33.6	34.3	0.0	0.0	81.8	261.2
NPL3	158.4	158.4	158.1	161.3	162.2	74.4	294.7
NPL4	-25.6	28.3	28.8	31.7	29.4	65.3	336.2

Table 5-2: GPS raw common clock differences, all values in ns.

Pair	RAW ΔC1	Sigma	RAW ΔP1	Sigma	RAW ΔP2	Sigma
TR-NPL1	-2.40	0.61	-2.89	0.69	-2.18	1.02
TR-NPL2	-37.22	0.61	-35.71	0.57	-36.01	1.06
TR-NPL3	-25.83	0.52	-23.45	0.56	-23.02	1.10
TR-NPL4	-31.83	0.62	-30.16	0.56	-30.15	0.91

Table 5-3: Galileo raw common clock differences, all values in ns.

Pair	RAW $\Delta E1$	Sigma	RAW $\Delta E5a$	Sigma
TR-NPL1	-	-	-	-
TR-NPL2	-38.66	0.48	-34.92	0.61
TR-NPL3	-25.82	0.53	-26.87	0.65
TR-NPL4	-33.07	0.44	-30.98	0.57

Taking a close loop to the closure measurements of Tables 5-4 and 5-5, we can observe a normal behavior of TR receiver, where the C1, P1, P2, E1 and E5a variations have remained relatively constant (below 0.35 ns).

Table 5-4: GPS closure measurements at ROA, all values in ns.

Pair	RAW $\Delta C1$	Sigma	RAW $\Delta P1$	Sigma	RAW $\Delta P2$	Sigma
TR-RO_9 (before the trip)	-0.02	0.41	-0.18	0.52	-0.07	0.63
TR-RO_9 (after the trip)	-0.25	0.47	-0.45	0.54	0.15	0.64
Misclosure	0.23		0.27		-0.22	
Mean	-0.14		-0.32		0.04	

Table 5-5: Galileo closure measurements at ROA, all values in ns.

Pair	RAW $\Delta E1$	Sigma	RAW $\Delta E5a$	Sigma
TR-RO_9 (before the trip)	-0.11	0.37	-0.08	0.39
TR-RO_9 (after the trip)	-0.12	0.40	0.36	0.45
Misclosure	0.01		-0.34	
Mean	-0.12		0.14	

6. UNCERTAINTY ESTIMATION

The overall uncertainty of the INT DLY values obtained as a result of the calibration is given by:

$$u_{CAL} = \sqrt{u_a^2 + u_b^2}, \quad (1)$$

with the statistical uncertainty u_a and the systematic uncertainty u_b . The statistical uncertainty is related to the instability of the common clock data collected at each site and collected at ROA when the INT DLY of travelling equipment was determined. The systematic uncertainty is given by:

$$u_b = \sqrt{\sum_n u_{b,n}^2} \quad (2)$$

The contributions to the sum (2) are listed and explained subsequently. In the Table 6-1, we have considered the larger type A uncertainty found at remote sites, which is quite small, so there is no need to develop it in detail for each Lab. Note that the uncertainty of the INT DLY values of ROA's fixed receiver RO_9, which served as the reference, is not included.

Table 6-1: Uncertainty contributions for the calibration of receiver delays

	Uncertainty	Value C1 ns	Value P1 ns	Value P2 ns	Value E1 ns	Value E5a ns	Description
1	$u_{a(ROA)}$	0.10	0.10	0.10	0.10	0.10	CCD uncertainty at ROA, TDEV at $\tau = 1$ day
1	$u_{a(NPL)}$	0.10	0.10	0.10	0.10	0.10	CCD uncertainty at remote Lab, TDEV at $\tau = 1$ day
Systematic components due to misclosure							
2	$u_{b,11}$	0.23	0.27	0.22	0.01	0.34	TR misclosure, see Tables 5-4 and 5-5
Systematic components due to antenna installation							
2	$u_{b,12}$	0.10	0.10	0.10	0.10	0.10	Position error of RO_9 receiver
3	$u_{b,13}$	0.10	0.10	0.10	0.10	0.10	Position error at remote Lab.
4	$u_{b,14}$	0.20	0.20	0.20	0.20	0.20	Multipath at ROA.
5	$u_{b,15}$	0.20	0.20	0.20	0.20	0.20	Multipath at remote Lab.
Installation of RO_9 and NPL receivers							
6	$u_{b,21}$	0.30	0.30	0.30	0.30	0.30	Connection of TR to UTC(ROA) (REF DLY).
7	$u_{b,22}$	0.50	0.50	0.50	0.50	0.50	Connection of TR to UTC(k) (REF DLY).
7	$u_{b,23}$	0.30	0.30	0.30	0.30	0.30	Connection of reference receiver to UTC(ROA) (REF DLY).
7	$u_{b,24}$	0.50	0.50	0.50	0.50	0.50	Connection of receivers at site k to UTC(k) (REF DLY).
7	$u_{b,25}$	0.10	0.10	0.10	0.10	0.10	TIC nonlinearities at ROA.
10	$u_{b,26}$	0.10	0.10	0.10	0.10	0.10	TIC nonlinearities at remote sites.

7. FINAL RESULTS

The results of the internal calibration are summarized in Table 7.1-2. INTDLY and associated uncertainty C1 values have been calculated from Table 5.1-3 and Table 6.1, respectively, rounded to the tenth of a nanosecond (the same for GPS P1, P2 and Galileo E1, E5a codes):

$$\text{INTDLY C1} = -\Delta\text{C1}(\text{Table 5-2/Table 5-3}) + \Delta\text{C1}_{\text{mean}}(\text{Table 5-4/Table 5-5})$$

Table 7-1: GPS calibration results, all values in ns.

Receiver	REF DLY	CAB DLY	INTDLY C1	u _{cal} C1	INT DLY P1	u _{cal} P1	INT DLY P2	u _{cal} P2
NPL1*	77.2	251.5	2.3	1.0	2.6	1.0	2.2	1.0
NPL2	81.8	261.2	37.1	1.0	35.4	1.0	36.0	1.0
NPL3	74.4	294.7	25.7	1.0	23.1	1.0	23.1	1.0
NPL4	65.3	336.2	31.7	1.0	29.8	1.0	30.2	1.0

* GTR50 INTDLY values are total values. Direct results of the calibration are changes with respect to the values previously entered in the receiver.

Table 7-2: Galileo calibration results, all values in ns.


Receiver	REF DLY	CAB DLY	INTDLY E1	u _{cal} E1	INT DLY E5a	u _{cal} E5a
NPL2	81.8	261.2	38.5	1.0	35.1	1.0
NPL3	74.4	294.7	25.7	1.0	27.0	1.0
NPL4	65.3	336.2	33.0	1.0	31.1	1.0

8. ANNEX-A

8.1. CALIBRATION INFORMATION SHEET AT ROA

Laboratory:	ROA	
Date and hour of the beginning of measurements:	24.07.2021	
Date and hour of the end of measurements:	28.07.2021	
Information on the system		
	Local:	Travelling:
4-character BIPM code	RO_9	TR
• Receiver maker and type:	Septentrio PolaRx4TR v2.9.2	Septentrio PolaRx5TR v5.3.2
Receiver serial number:	3102314	4701310
1 PPS trigger level /V:	1 V	1 V
• Antenna cable maker and type:	LDF1RK-50	H155
Phase stabilised cable (Y/N):		
Length outside the building /m:	Approximately 37 m	Approximately 50 m
• Antenna maker and type:	LEICA AR25	Novatel antenna GPS-703-GGG
Antenna serial number:	725232	01018146
Measured delays /ns		
	Local:	Travelling:
• Delay from local UTC to receiver 1 PPS-in:	305.6 ns	295.5 ns Auto-compensation PPS IN: ON
Delay from 1 PPS-in to internal Reference (if different): <small>(see section 2 for details)</small>	146.2 ns	
• Total reference delay:	451.8 ns	
• Antenna cable delay:	59.7 ns	259.6 ns
Antenna cable type:		
Data used for the generation of CGGTTS files		
	Local:	Travelling:
• INT DLY (GPS) /ns:	56.3 ns C1, 54.9 ns P1, 54.0 ns P2	28.4 ns C1, 26.2 ns P1, 25.6 ns P2
• INT DLY (GALILEO) /ns:	55.8 ns E1, 64.7 ns E5a	28.4 ns E1, 27.6 ns E5a
• CAB DLY /ns:	59.7 ns	259.6 ns
• REF DLY /ns:	451.8 ns	295.5 ns
• Coordinates reference frame:	ITRF	ITRF
Latitude or X /m:	5105582.90 m	5105579.90 m
Longitude or Y /m:	-555191.22 m	-555190.14 m
Height or Z /m:	3769703.66 m	3769707.61 m
General information		
• Rise time of the local UTC pulse:	0.5 ns	
• Is the laboratory air conditioned:	Yes	
Set temperature value and uncertainty:	(22 ± 2) °C	
Set humidity value and uncertainty:	< 70 %	


Diagram of the experiment set-up:

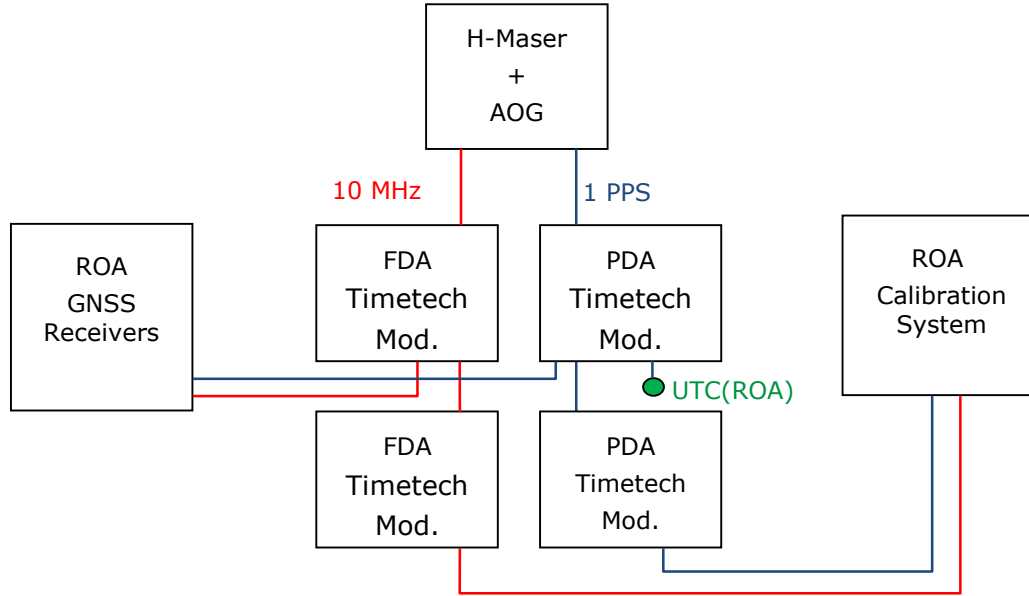

8.2. CALIBRATION INFORMATION SHEET AT NPL


Laboratory:	NPL	
Date and hour of the beginning of measurements:	12.10.2021	
Date and hour of the end of measurements:	17.10.2021	
Information on the system		
	Local:	Travelling:
4-character BIPM code	NPL1	TR
• Receiver maker and type:	DICOM GTR50	Septentrio PolaRx5TR v5.3.2
Receiver serial number:	0807183	4701310
1 PPS trigger level /V:	1 V	1 V
• Antenna cable maker and type:	Andrew Helix FSJ1-50A cable	H155
Phase stabilised cable (Y/N):	Y	
Length outside the building /m:	Approximately 6 m (plus approximately 30 m in a roof space with no T. control)	Approximately 50 m
• Antenna maker and type:		Novatel antenna GPS-703-GGG
Antenna serial number:	Novatel GPS-702	01018146
Measured delays /ns		
	Local:	Travelling:
• Delay from local UTC to receiver 1 PPS-in:	77.2 ns	69.5 ns Auto-compensation PPS IN: ON
Delay from 1 PPS-in to internal Reference (if different): <small>(see section 2 for details)</small>		
• Total delay:		
• Antenna cable delay:	251.5 ns	259.6 ns
Antenna cable type:		
Data used for the generation of CGGTTS files		
	Local:	Travelling:
• INT DLY (GPS) /ns:	-37.2 ns C1, -37.9 ns P1, -29.0 ns P2	28.4 ns C1, 26.2 ns P1, 25.6 ns P2
• INT DLY (GALILEO) /ns:	0 ns E1, 0 ns E5a	28.4 ns E1, 27.6 ns E5a
• CAB DLY /ns:	251.5 ns	259.6 ns
• REF DLY /ns:	77.2 ns	69.5 ns
• Coordinates reference frame:	ITRF	ITRF
Latitude or X /m:	3985120.13 m	3985110.09 m
Longitude or Y /m:	-23893.65 m	-23888.87 m
Height or Z /m:	4963240.40 m	4963248.40 m
General information		
• Rise time of the local UTC pulse:		0.5 ns
• Is the laboratory air conditioned:		Yes
Set temperature value and uncertainty:		(22 ± 2) °C
Set humidity value and uncertainty:		< 70 %

Diagram of the experiment set-up:

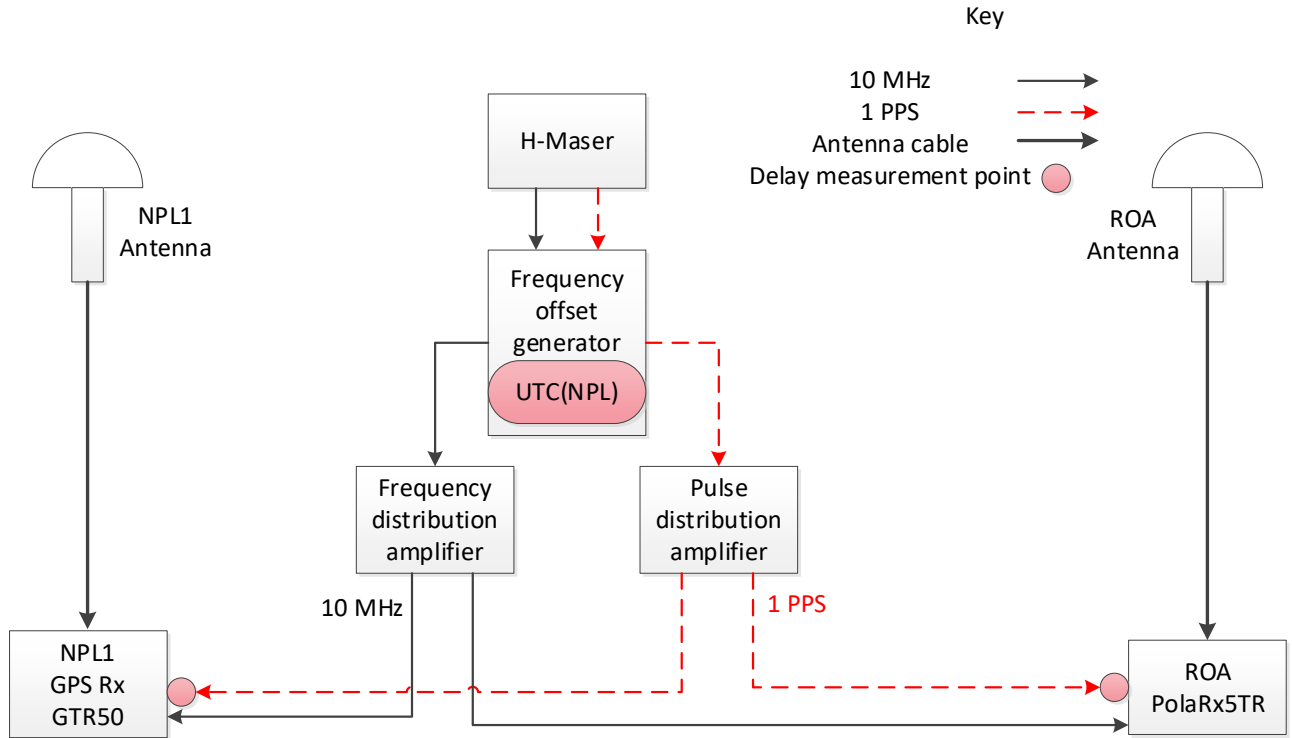


Laboratory:	NPL	
Date and hour of the beginning of measurements:	12.10.2021	
Date and hour of the end of measurements:	17.10.2021	
Information on the system		
	Local:	Travelling:
4-character BIPM code	NPL2	TR
• Receiver maker and type:	MESIT GTR51	Septentrio PolaRx5TR v5.3.2
Receiver serial number:	1401406	4701310
1 PPS trigger level /V:	1 V	1 V
• Antenna cable maker and type:	Andrew Helix FSJ1-50A cable	H155
Phase stabilised cable (Y/N):	Y	
Length outside the building /m:	Approximately 4 m (plus approximately 30 m in a roof space with no T. control)	Approximately 50 m
• Antenna maker and type:		Novatel antenna GPS-703-GGG
Antenna serial number:	Novatel GPS-702	01018146
Measured delays /ns		
	Local:	Travelling:
• Delay from local UTC to receiver 1 PPS-in:	81.8 ns	69.5 ns Auto-compensation PPS IN: ON
Delay from 1 PPS-in to internal Reference (if different): <small>(see section 2 for details)</small>		
• Total delay:		
• Antenna cable delay:	261.2 ns	259.6 ns
Antenna cable type:		
Data used for the generation of CGGTTS files		
	Local:	Travelling:
• INT DLY (GPS) /ns:	35.7 ns C1, 33.6 ns P1, 34.3 ns P2	28.4 ns C1, 26.2 ns P1, 25.6 ns P2
• INT DLY (GALILEO) /ns:	0 ns E1, 0 ns E5a	28.4 ns E1, 27.6 ns E5a
• CAB DLY /ns:	261.2 ns	259.6 ns
• REF DLY /ns:	81.8 ns	69.5 ns
• Coordinates reference frame:	ITRF	ITRF
Latitude or X /m:	3985118.08 m	3985110.09 m
Longitude or Y /m:	-23892.66 m	-23888.87 m
Height or Z /m:	4963242.04 m	4963248.40 m
General information		
• Rise time of the local UTC pulse:		0.5 ns
• Is the laboratory air conditioned:		Yes
Set temperature value and uncertainty:		(22 ± 2) °C
Set humidity value and uncertainty:		< 70 %

Diagram of the experiment set-up:

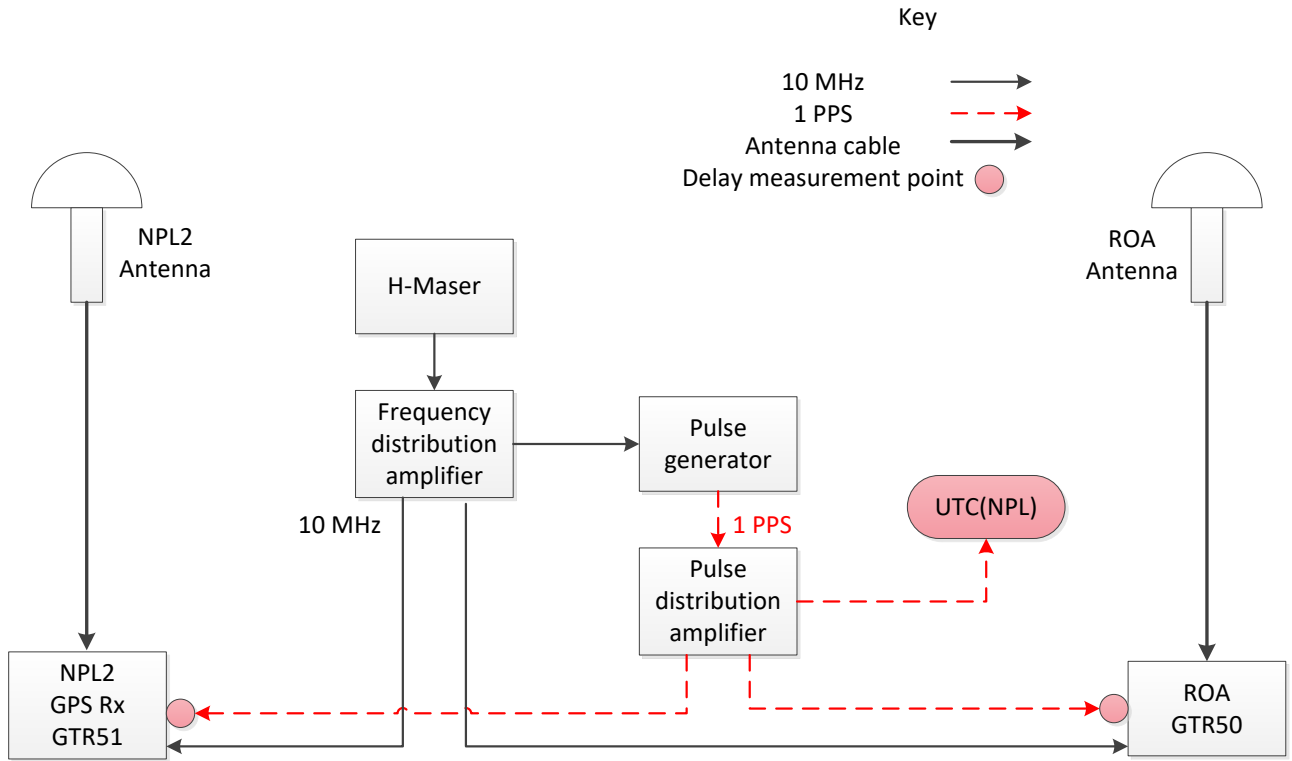


Laboratory:	NPL	
Date and hour of the beginning of measurements:	12.10.2021	
Date and hour of the end of measurements:	17.10.2021	
Information on the system		
	Local:	Travelling:
4-character BIPM code	NPL3	TR
• Receiver maker and type: Receiver serial number:	Septentrio PolaRx5TR 4701299	Septentrio PolaRx5TR v5.3.2 4701310
1 PPS trigger level /V:	1 V	1 V
• Antenna cable maker and type: Phase stabilised cable (Y/N):	Andrew Heliax FSJ1-50A cable Y	H155
Length outside the building /m:	Approximately 4 m (plus approximately 30 m in a roof space with no T. control)	Approximately 50 m
• Antenna maker and type: Antenna serial number:		Novatel antenna GPS-703-GGG 01018146
Measured delays /ns		
	Local:	Travelling:
• Delay from local UTC to receiver 1 PPS-in:	74.4 ns Auto-compensation PPS IN: ON	69.5 ns Auto-compensation PPS IN: ON
Delay from 1 PPS-in to internal Reference (if different): <small>(see section 2 for details)</small>		
• Total delay:		
• Antenna cable delay: Antenna cable type:	294.7 ns	259.6 ns
Data used for the generation of CGGTTS files		
	Local:	Travelling:
• INT DLY (GPS) /ns:	158.4 ns C1, 158.4 ns P1, 158.1 ns P2	28.4 ns C1, 26.2 ns P1, 25.6 ns P2
• INT DLY (GALILEO) /ns:	161.3 ns E1, 162.2 ns E5a	28.4 ns E1, 27.6 ns E5a
• CAB DLY /ns:	294.7 ns	259.6 ns
• REF DLY /ns:	74.4 ns	69.5 ns
• Coordinates reference frame:	ITRF	ITRF
Latitude or X /m:	3985114.22 m	3985110.09 m
Longitude or Y /m:	-23890.83 m	-23888.87 m
Height or Z /m:	4963245.10 m	4963248.40 m
General information		
• Rise time of the local UTC pulse:		0.5 ns
• Is the laboratory air conditioned:		Yes
Set temperature value and uncertainty:		(22 ± 2) °C
Set humidity value and uncertainty:		< 70 %

Diagram of the experiment set-up:

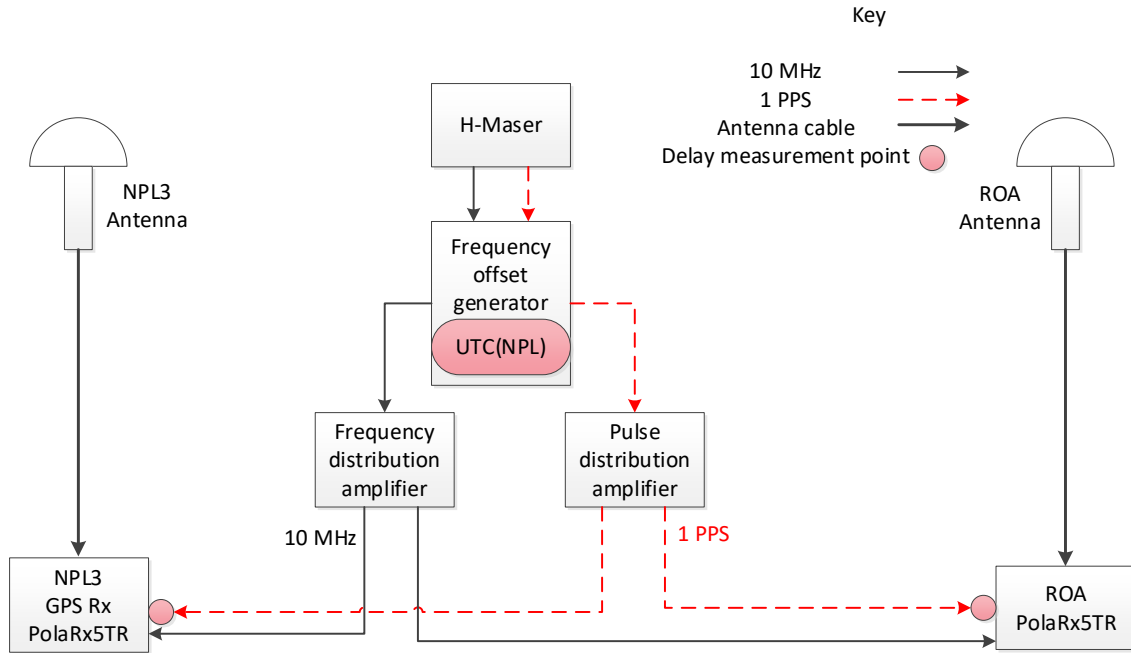

Laboratory:	NPL	
Date and hour of the beginning of measurements:	12.10.2021	
Date and hour of the end of measurements:	17.10.2021	
Information on the system		
	Local:	Travelling:
4-character BIPM code	NPL4 File names are GAL1	TR
• Receiver maker and type: Receiver serial number:	MESIT GTR51 1611078	Septentrio PolaRx5TR v5.3.2 4701310
1 PPS trigger level /V:	1 V	1 V
• Antenna cable maker and type: Phase stabilised cable (Y/N):	Andrew Heliac FSJ1-50A cable Y	H155
Length outside the building /m:	Approximately 4 m (plus approximately 30 m in a roof space with no T. control)	Approximately 50 m
• Antenna maker and type: Antenna serial number:	NOV-703-GGG NEG 16290013	Novatel antenna GPS-703-GGG 01018146
Measured delays /ns		
	Local:	Travelling:
• Delay from local UTC to receiver 1 PPS-in:	65.3 ns	69.5 ns Auto-compensation PPS IN: ON
Delay from 1 PPS-in to internal Reference (if different): <small>(see section 2 for details)</small>		
• Total delay:		
• Antenna cable delay: Antenna cable type:	336.2 ns	259.6 ns
Data used for the generation of CGGTTS files		
	Local:	Travelling:
• INT DLY (GPS) /ns:	-25.6 ns C1, 28.3 ns P1, 28.8 ns P2	28.4 ns C1, 26.2 ns P1, 25.6 ns P2
• INT DLY (GALILEO) /ns:	31.7 ns E1, 29.4 ns E5a	28.4 ns E1, 27.6 ns E5a
• CAB DLY /ns:	336.2 ns	259.6 ns
• REF DLY /ns:	65.3 ns	69.5 ns
• Coordinates reference frame:	ITRF	ITRF
Latitude or X /m:	3985112.18 m	3985110.09 m
Longitude or Y /m:	-23889.85 m	-23888.87 m
Height or Z /m:	4963246.76 m	4963248.40 m
General information		
• Rise time of the local UTC pulse:		0.5 ns
• Is the laboratory air conditioned:		Yes
Set temperature value and uncertainty:		(22 ± 2) °C
Set humidity value and uncertainty:		< 70 %

Diagram of the experiment set-up:

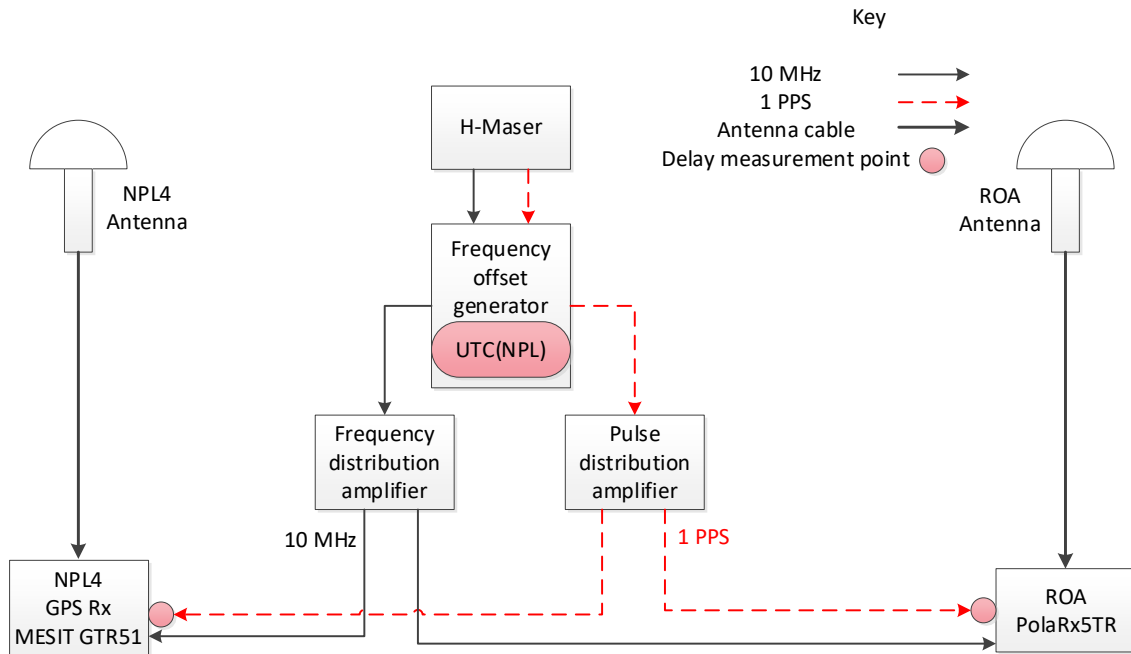

9. ANNEX-B: CCD at each Lab

Figure 9-1: Before the calibration trip (GPS)

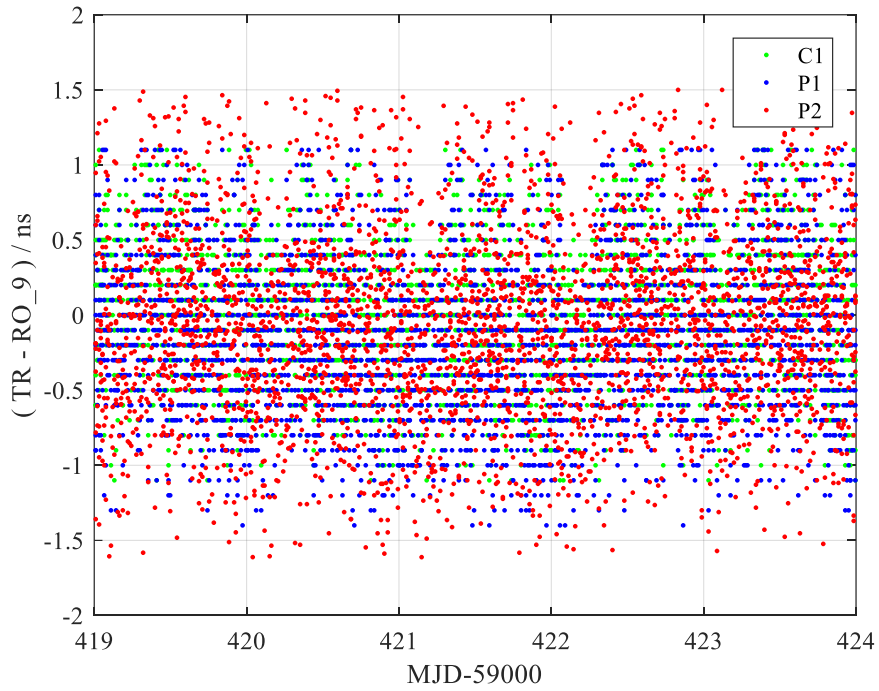


Figure 9-2: Before the calibration trip (Galileo)

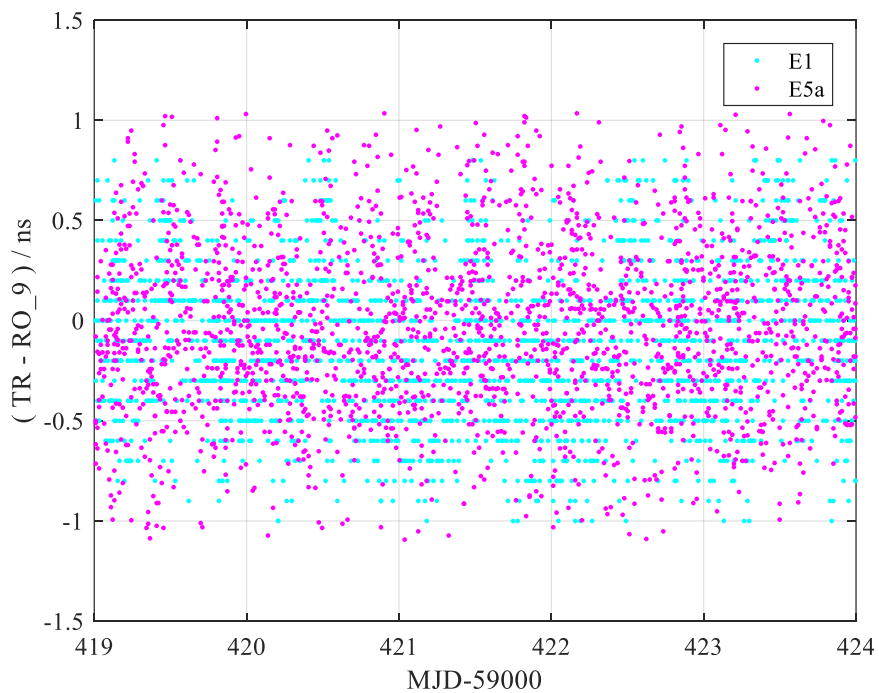


Figure 9-3: After the calibration trip (GPS)

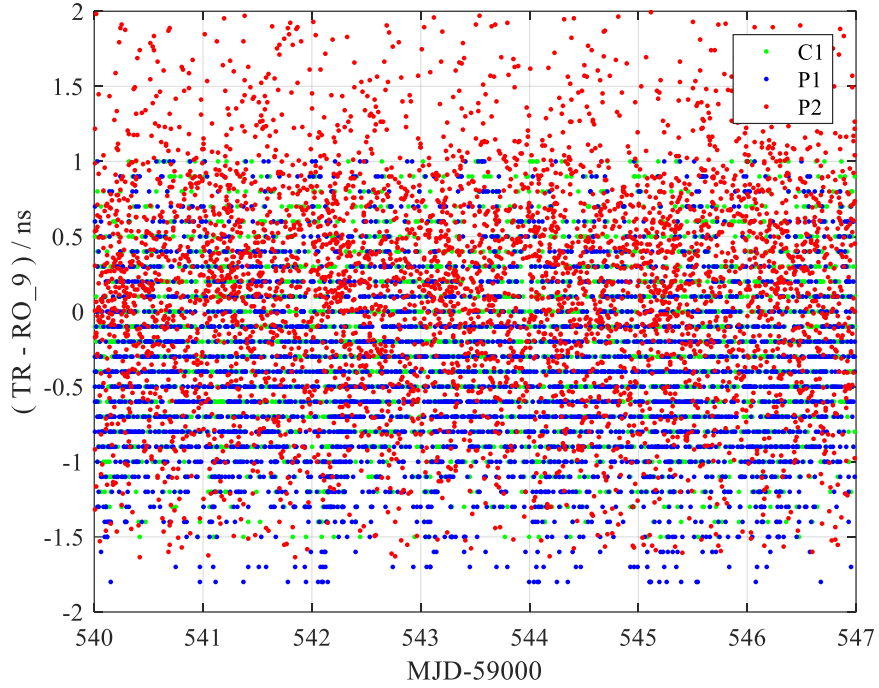


Figure 9-4: After the calibration trip (Galileo)

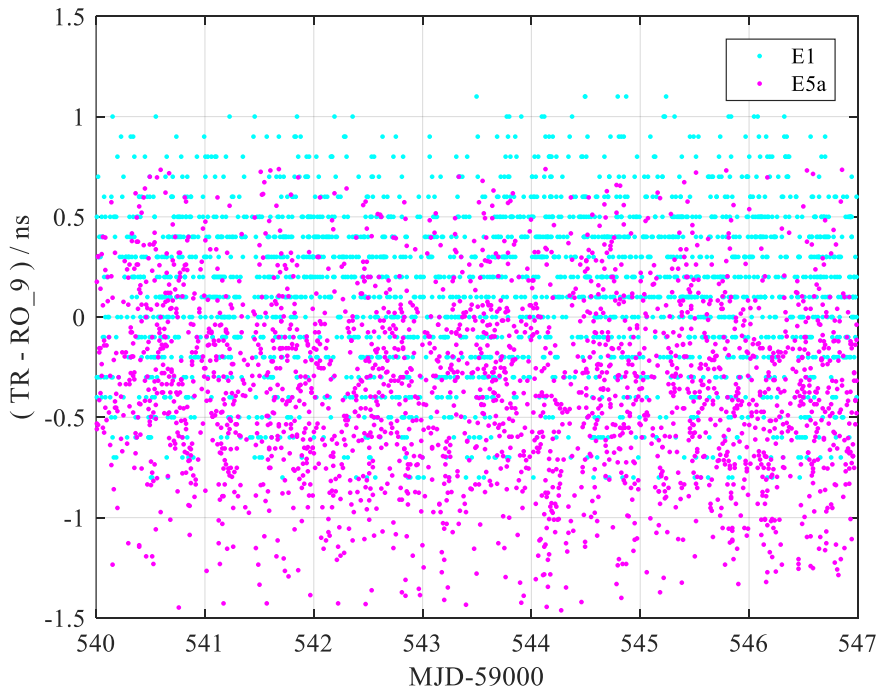
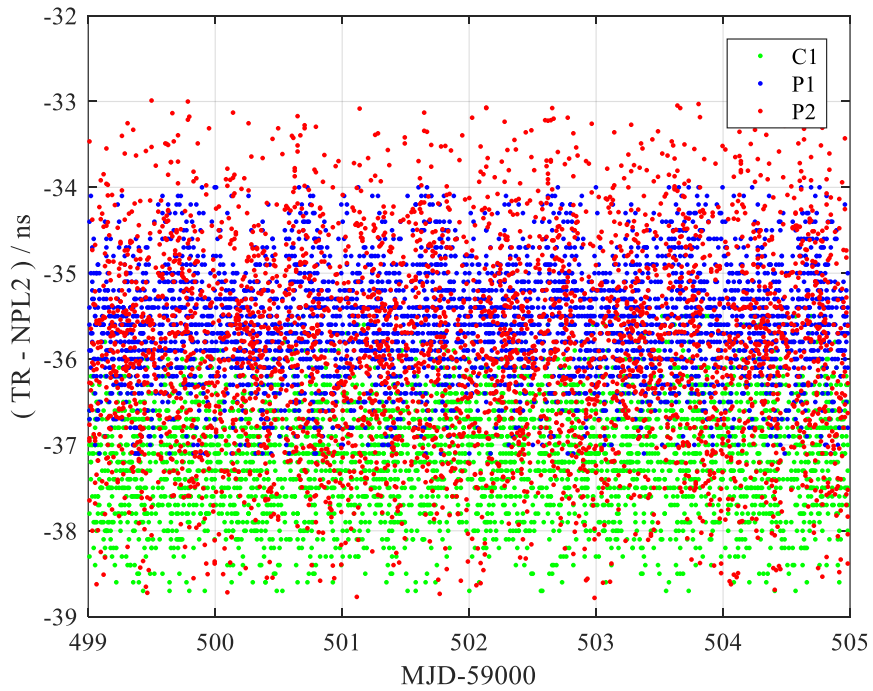
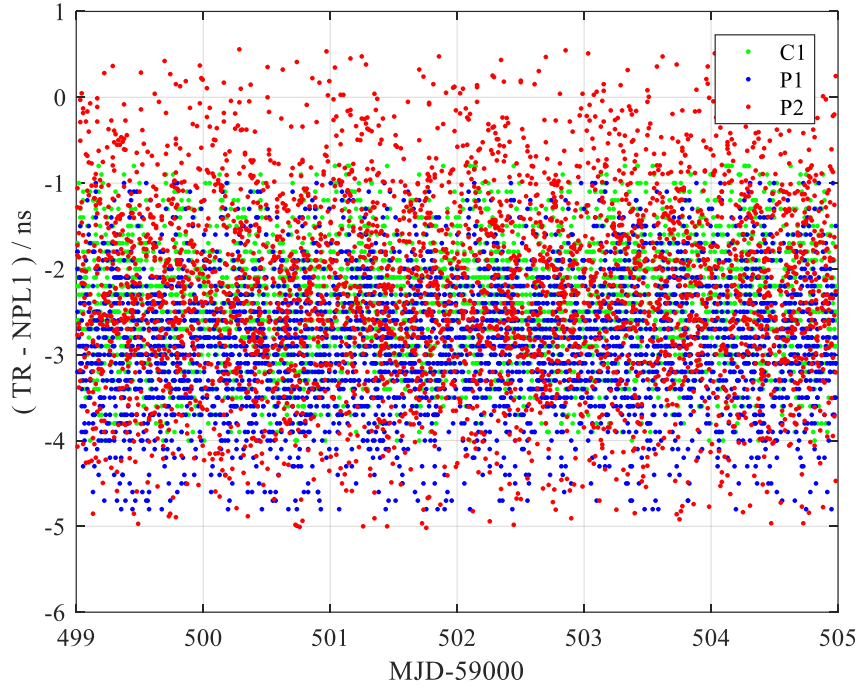


Figure 9-5: GPS CCD at NPL






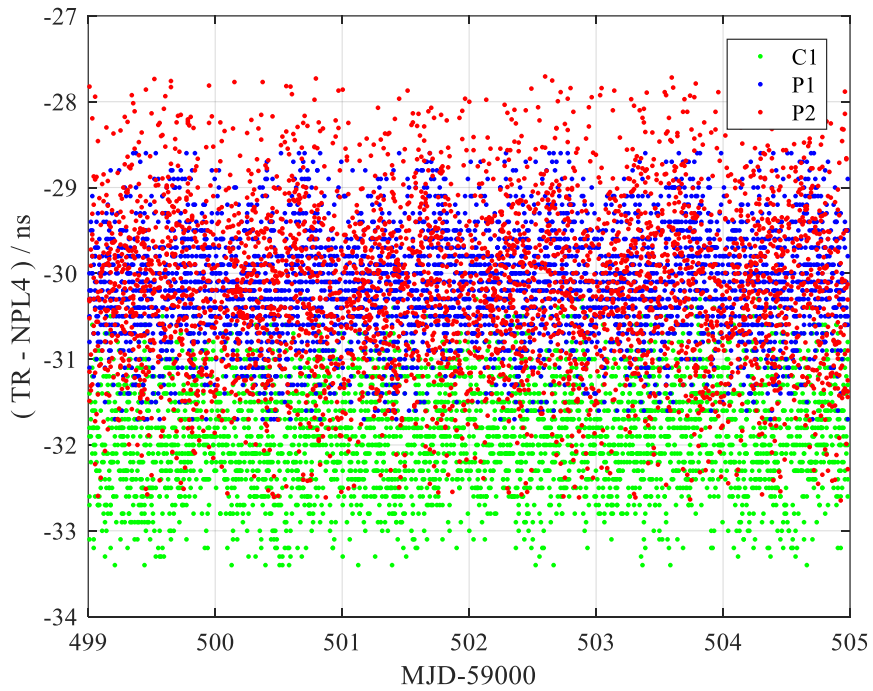


Figure 9-6: Galileo CCD at NPL

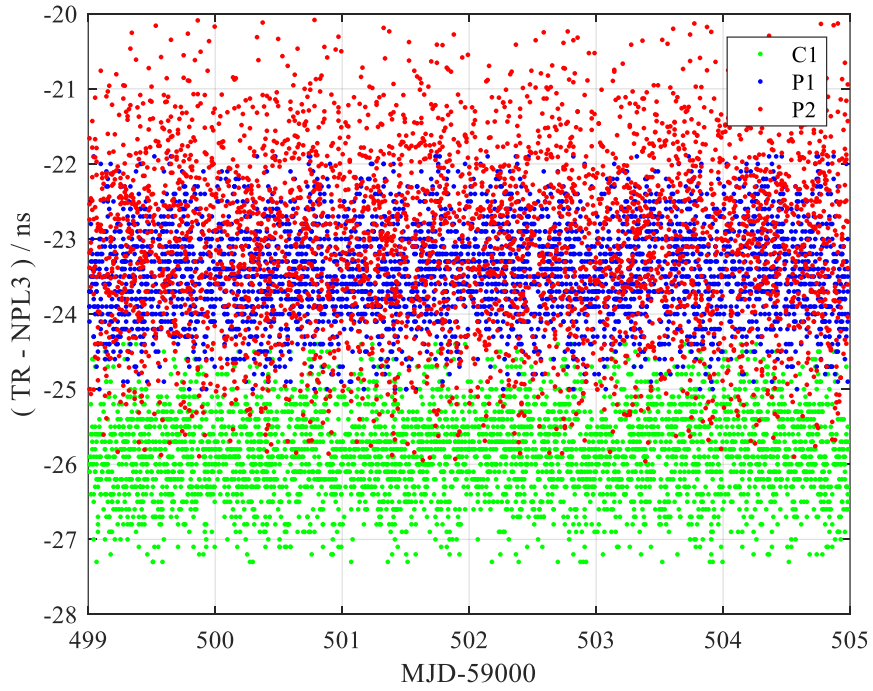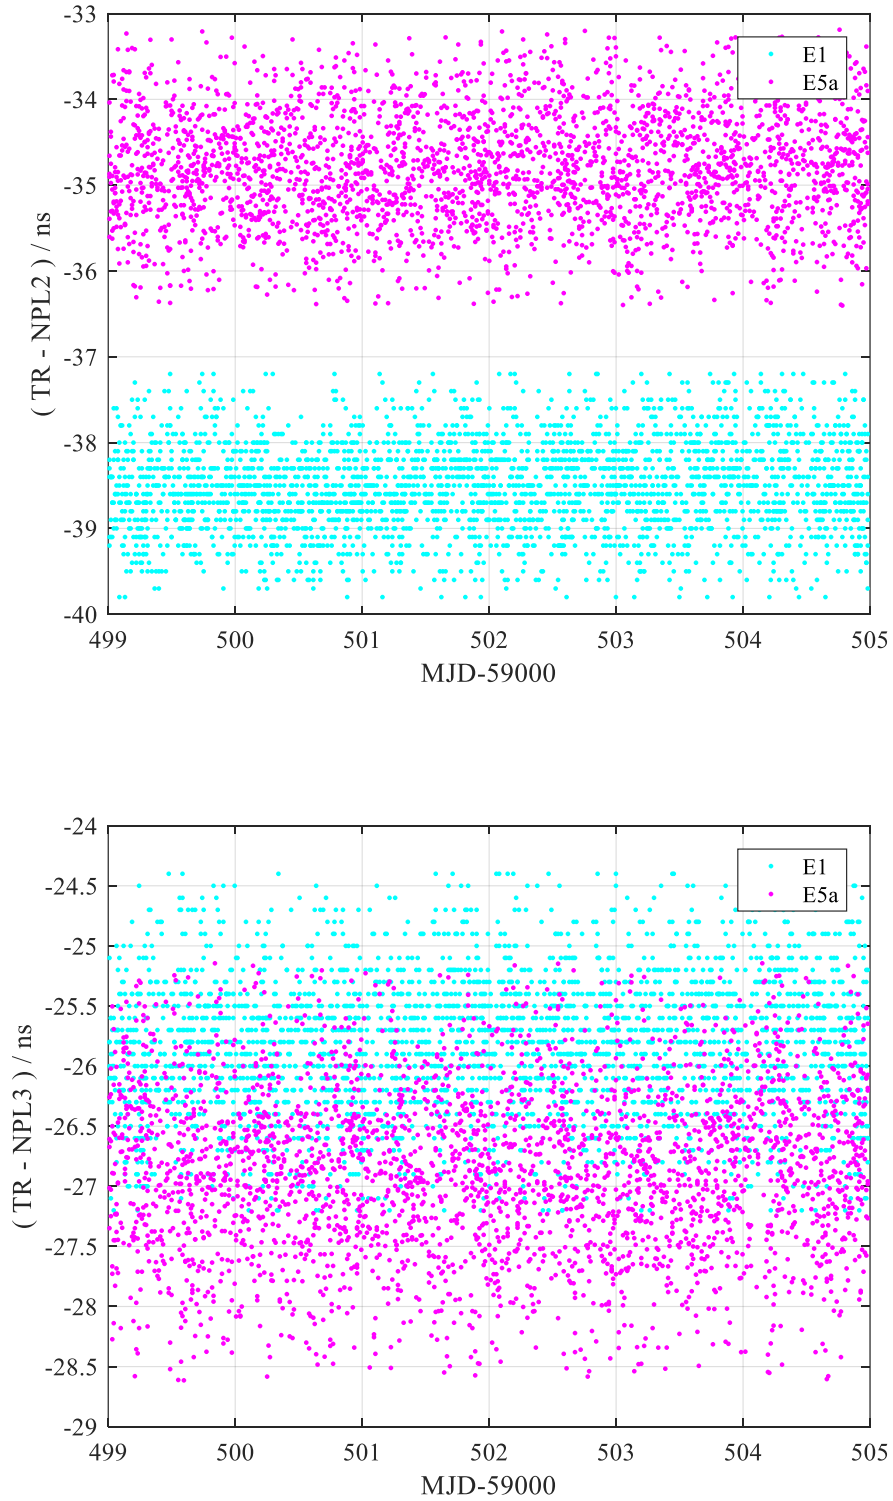

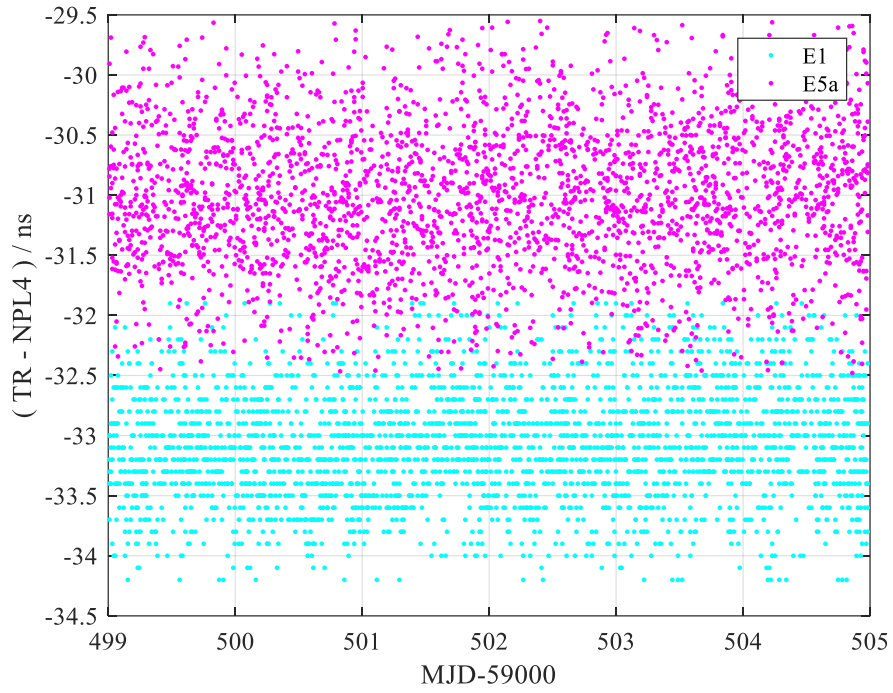

Acknowledgement

We are grateful to the Natural Resources Canada (NRCan) for the use of Precise Point Positioning (PPP) software for positioning computations.

Special thanks to our colleagues Peter Whibberley and Elizabeth Laier from NPL for the unreserved collaboration and support he has provided.

END OF DOCUMENT